

INSTITUT FRESNEL

PATRICK C. CHAUMET


DANIEL SENTENAC

ANNE SENTENAC

IF-DDAM

Idiot Friendly-Discrete Dipole Approximation for Multilayer

version : 0.8.2

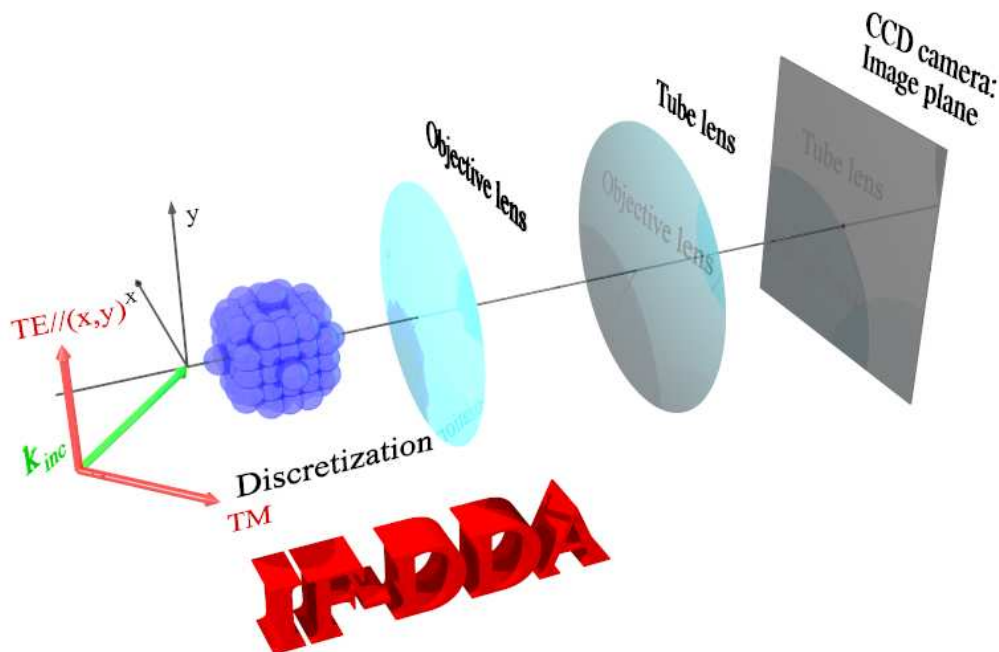

Contents

List of figures	v
1 Generality	1
1.1 Introduction	1
1.2 The principle of discrete dipole approximation in a multilayer system	2
1.3 A word about the code	3
1.4 How to compile the code	3
1.5 A word about the authors	4
1.6 Licence	4
1.7 How to quote the code	4
2 Approximation to increase the efficiency of the code	5
2.1 Introduction	5
2.2 Approximated method	7
2.2.1 Born	7
2.2.2 Renormalized Born	7
2.2.3 Born at the order 1	7
2.2.4 Scalar Approximation revisited	7
2.3 Computation of the Green function	8
3 Numerical details	9
3.1 Polarizability	9
3.2 Solve the system of linear equation	10
3.3 Change of the initial guess	11
3.4 Preconditioning the system of linear equations	11
3.5 The default options and how to change them	11
4 Managing of the configurations	13
4.1 Introduction	13
4.2 Creation and saving of a new configuration	13
4.3 Managing of the configurations	13
5 Properties of the illumination	14
5.1 Introduction	14
5.2 Beam	14
5.2.1 Introduction	14
5.2.2 Linear plane wave	15

5.2.3	Circular plane wave	16
5.2.4	Multiple plane wave	16
5.2.5	Linear Gaussian beam	16
5.2.6	Circular Gaussian	16
5.2.7	Speckle	17
5.2.8	Antenna	17
5.2.9	Arbitrary wave	18
6	Properties of the multilayer	20
6.1	Introduction	20
6.2	Remarks	21
7	Definition of the object	22
7.1	Introduction	22
7.2	Type of the object	22
7.2.1	Sphere	23
7.2.2	Inhomogeneous sphere	23
7.2.3	Cube	24
7.2.4	Cuboid (length)	24
7.2.5	Cuboid (meshsize)	24
7.2.6	Inhomogeneous Cuboid (length)	25
7.2.7	Inhomogeneous Cuboid (meshsize)	25
7.2.8	Ellipsoid	25
7.2.9	Multiple spheres	26
7.2.10	Cylinder	26
7.2.11	Concentric spheres	26
7.2.12	Arbitrary object	26
7.3	Choose the relative permittivity	27
7.4	Choose the discretization	28
8	Possible study with the code	29
8.1	Introduction	29
8.2	Study in far field	29
8.3	Microscopy	31
8.4	Study in near field	32
9	Representation of the results	34
9.1	Introduction	34
9.2	Digital exits	34
9.3	Graphics	35
9.3.1	Plot epsilon/dipoles	35
9.3.2	Far field and microscopy	35
9.3.2.1	Plot Poynting vector	35
9.3.2.2	Plot microscopy	35
9.3.3	Study of the near field	36
10	Ouput files for matlab, octave, scilab,...	37
10.1	Introduction	37
10.2	List of all exit files	38

11 Some examples	41
11.1 Introduction	41
11.2 Test1	41
11.3 Test2	45
11.4 Test3	49
11.5 Test4	51
Bibliography	54

List of Figures

1.1	Principle of the DDA : the object under study (on the left) is discretized in a set of small dipoles (on the right)l.	2
5.1	Definition of the beam's direction	15
5.2	Definition of the beam's polarization.	15
5.3	(a) Configuration: Antenna in a vacuum above an interface of permittivity $\epsilon = 20$ (b) Total radiated power versus the distance from the antenna to the interface. (c) Lifetime of a fluorescent atom as a function of its distance from the interface.	18
6.1	How to configure the layer.	20
7.1	Definition of the angles of Euler according to the convention $Z - X - Z$. Scheme taken from Wikipedia	23
8.1	Simplified figure of the microscope. The object focus of the objective lens are at the origin of the frame but can be changed. The axis of the lens is confounded with the z axis.	31
11.1	Test1: configuration taken.	42
11.2	Modulus of the local field in (x, y) plane.	42
11.3	Modulus of the macroscopic field in (x, y) plane.	43
11.4	Modulus of the Poynting vector.	43
11.5	Modulus of the diffracted field in the Fourier plane in transmission (left) and in reflection (right) for optical diffraction microscope.	44
11.6	Modulus of the field in the image plane in transmission (left) and in reflection (right) for optical diffraction tomography. Diffracted field (above) and total field (below).	44
11.7	Test2: configuration taken.	45
11.8	Test2: relative permittivity. Real part (left) and imaginary part (right). . .	46
11.9	Modulus of the local field in the (x, y) plane.	46
11.10	Modulus of the macroscopic field in the (x, y) plane.	47
11.11	Modulus of the Poynting vector.	47
11.12	Modulus of the field in the Fourier plane in transmission (left) and in reflection (right) for an optical diffraction tomography microscope. Diffracted field (above) and total field (below).	48

11.13	Modulus of the field in the image plane in transmission (left) and in reflection (right) for an optical diffraction tomography microscope. Diffracted field (above) and total field (below).	49
11.14	Test3: configuration taken.	50
11.15	Test3: Incident field used to simulate the microscope.	50
11.16	Modulus of the field in the image plane in case of transmission (left) and reflection (right) for a darkfield (above) and brightfield (below) microscope.	51
11.17	Test3: configuration taken.	52
11.18	Test4: Incident field used to simulate the microscope.	52
11.19	Modulus of the field in the image plane in case of transmission (left) and reflection (right) for a darkfield (above) and phase (below) microscope.	53

Generality

Contents

1.1	Introduction	1
1.2	The principle of discrete dipole approximation in a multilayer system	2
1.3	A word about the code	3
1.4	How to compile the code	3
1.5	A word about the authors	4
1.6	Licence	4
1.7	How to quote the code	4

1.1 Introduction

This software computes the diffraction of an electromagnetic wave by a three-dimensional object in a multilayer system. This interaction is taken into account rigorously by solving the Maxwell's equations, but can also do with the approximation of Born at the order 0 or 1. The code has an user-friendly interface and allows you to choose canonical objects (sphere, cube, ...) as well as predefined incident waves (plane wave, Gaussian beam, ...) or arbitrary objects and incidents waves. After by drop-down menus, it is easy to study cross sections, diffraction near field and far field as well as microscopy in transmission or reflection (holography, brighthfield, dark field,...).

There are numerous methods that enable the study of the diffraction of an electromagnetic wave by an object of arbitrary form and relative permittivity. We are not going here to set up an exhaustive list of these methods, but the curious reader may refer to the article by F. M. Kahnert who details the advantages and weaknesses of the most common methods.¹

The method we use is called coupled dipoles method (CDM) or the discrete dipole approximation (DDA). This method is a volume method, because the diffracted field is obtained from an integral, the support of which is the volume of the considered object. It had been introduced by E. M. Purcell and C. R. Pennypacker in 1973, in order to study the scattering of light by grains in interstellar medium.²

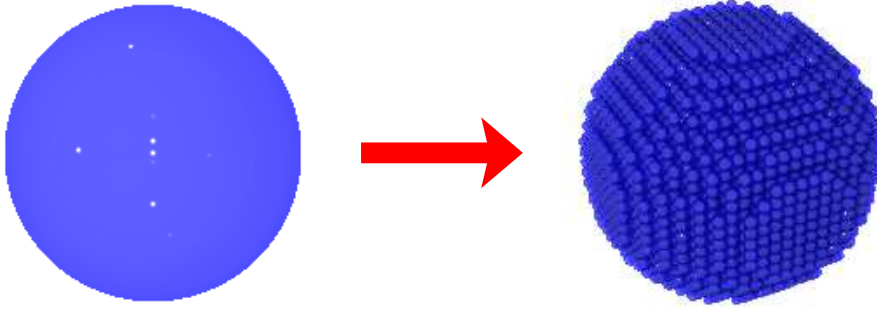


Figure 1.1 : *Principle of the DDA : the object under study (on the left) is discretized in a set of small dipoles (on the right).*

1.2 The principle of discrete dipole approximation in a multilayer system

Take an object of arbitrary form and relative permittivity in a multilayer system. This multilayer is submitted to a incident field electromagnetic wave of wavelength λ ($k_0 = 2\pi/\lambda$). In the absence of the object under study a reference field takes place in the multilayer. The principle of the DDA consists in representing the object as a set of N small cubes of an edge a [by little, we mean smaller than the wavelength in the object : $a \ll \lambda/\sqrt{\epsilon}$ (Fig. 1.1)]. Each one of the small cubes under the action of the reference wave is going to get polarized, and as such, to acquire a dipolar moment, whose value is going to depend on the reference field and on its interaction with its neighbours. The local field of a dipole located at \mathbf{r}_i , $\mathbf{E}(\mathbf{r}_i)$, is the sum of the incident wave and the field radiated by the dipoles :

$$\mathbf{E}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \mathbf{G}(\mathbf{r}_i, \mathbf{r}_j) \alpha(\mathbf{r}_j) \mathbf{E}(\mathbf{r}_j). \quad (1.1)$$

\mathbf{E}_{ref} is the reference wave, \mathbf{G} the linear susceptibility of the field of the multilayer system. α is the polarizability of each discretization element obtained from the Clausius-Mossotti relation. Note that the polarizability α , in order to respect the optical theorem, needs to contain a term called the radiative reaction term.³ Equation (1.1) is valid for $i = 1, \dots, N$, and so represents a system of $3N$ linear equations where the local fields, $\mathbf{E}(\mathbf{r}_i)$, being the unknowns. Once the system of linear equation is solved, the field scattered by the object at an arbitrary position \mathbf{r} is obtained by making the sum of all the radiated fields by each one of the dipoles :

$$\mathbf{E}(\mathbf{r}) = \sum_{j=1}^N \mathbf{G}(\mathbf{r}, \mathbf{r}_j) \alpha(\mathbf{r}_j) \mathbf{E}(\mathbf{r}_j). \quad (1.2)$$

We have just presented the DDA as E. M. Purcell and C. R. Pennypacker had presented it earlier.² Note that another method very close to the DDA does exist. This method called the method of the moments starts from the integral equation of Lippman Schwinger, which is strictly identical to the DDA. The demonstration of the equivalence between these two methods being a little technical, it is explained in Ref.⁴.

The advantages of the DDA are that it is applicable to objects of arbitrary forms, inhomogeneous (that is hardly achievable in case of surface method), and anisotropic (the polarizability associated to the mesh becomes a tensor). The outgoing wave condition is automatically satisfied through the linear susceptibility of the field. Finally, note that only the object is discretized unlike the methods of finite differences and finite elements.¹ The main inconvenience of the DDA consists in the fast increase of computation time together with the increase of the number of discretization elements, *i.e.*, the increase in size of the system of linear equations to be solved.

1.3 A word about the code

The code is thought to have a user-friendly interface so that everyone can use it without any problems including non specialists. This allows undergraduate students to study, for example, the basics of microscopy (Rayleigh's criteria, notion of numerical aperture, ...) or diffraction without any problem; and researchers, typically biologists, having no notion of Maxwell's equations to simulate what gives a microscope (brightfield, phase microscope, dark field, ...) in function of the usual parameters and the object. Nevertheless, this code can also serve physicists specializing in electromagnetism in performing, for example, calculations of diffraction, cross sections, near field and this with many incident beams.

The code thus has by default a simple interface where all numerical parameters are hidden and where many options are then chosen by default. But it's easy to access all Code options by checking the Advanced Interface option. This user guide explains how to use the advanced interface in starting with the different approaches used by the code to solve the Maxwell equations.

Note that the usability of the code is made to the detriment of the optimization of the RAM and the code can use large memory for large objects.

1.4 How to compile the code

The application is based on Qt-4.8 and gfortran. To install it you need : qt, qt-devel, gcc-c++ et gfortran. Notice that there are three versions of the code, the first one is sequential and uses FFTE (Fast Fourier Transform in the east), the second one uses FFTW (Fast Fourier Transform in the west) which needs openmp 4.5 minimum and the third uses HDF5 format to save data file. Currently according to the age of the linux you use, you have Qt4 or Qt5. The code has been tested under the two environments, but to compile you need adapt qt4 in qt5 on recent versions, I will note for make compact qt4(5). Then to compile:

Code par défaut	Code avec FFTW	Code avec FFTW et HDF5
qmake-qt4(5) make make install	qmake-qt4(5) "CONFIG+=fftw" make make install	qmake-qt4(5) "CONFIG+=fftw hdf5" make make install

To run the application, cd bin, and ./cdm.

On linux system with the library FFTW, it requires to install FFTW packages with "dnf install * fftw *". For the version that uses HDF5 file you should install the following packages "dnf install hdf hdf5 hdf5-static hdf5-devel".

The code works on windows system but it is tricky to compile it if you want to use FFTW.

1.5 A word about the authors

- P. C. Chaumet is Professor at Fresnel Institute of Aix-Marseille University, and deals with the development of the fortran source code.
- A. Sentenac is research director at the CNRS, and works at Fresnel Institute of Aix-Marseille University, and participates to the development of the code connected to the far field diffraction.
- D. Sentenac of European Gravitational Observatory in Italia develops the convivial interface of the code.

1.6 Licence

Attribution-NonCommercial-ShareAlike 4.0 International (CC BY-NC-SA 4.0)

You are free to:

- Share - copy and redistribute the material in any medium or format
- Adapt - remix, transform, and build upon the material

The licensor cannot revoke these freedoms as long as you follow the license terms.

- Attribution - You must give appropriate credit, provide a link to the license, and indicate if changes were made. You may do so in any reasonable manner, but not in any way that suggests the licensor endorses you or your use.
- NonCommercial - You may not use the material for commercial purposes.
- ShareAlike - If you remix, transform, or build upon the material, you must distribute your contributions under the same license as the original.

1.7 How to quote the code

- P. C. CHAUMET, D. SENTENAC, G. MAIRE, M. RASEDUJJAMAN, T. ZHANG and A. SENTENAC,
IFDDA, an easy-to-use code for simulating the field scattered by 3D inhomogeneous objects in a stratified medium: tutorial.
J. Opt. Soc. Am. A **38**, 1841 (2021).
- S. KHADIR, P. C. CHAUMET, G. BAFFOU and A. SENTENAC,
Quantitative model of the image of a radiating dipole through a microscope.
J. Opt. Soc. Am. A **36**, 478 (2019).

Approximation to increase the efficiency of the code

Contents

2.1 Introduction	5
2.2 Approximated method	7
2.2.1 Born	7
2.2.2 Renormalized Born	7
2.2.3 Born at the order 1	7
2.2.4 Scalar Approximation revisited	7
2.3 Computation of the Green function	8

2.1 Introduction

In the previous chapter we have presented the DDA in a simple way where the object under study is a set of radiating dipole. In an approach more rigorous, with the Maxwell's equation, we get in Gaussian unit:

$$\nabla \times \mathbf{E}^m(\mathbf{r}) = i\frac{\omega}{c}\mathbf{B}(\mathbf{r}) \quad (2.1)$$

$$\nabla \times \mathbf{B}(\mathbf{r}) = -i\frac{\omega}{c}\varepsilon(\mathbf{r})\mathbf{E}^m(\mathbf{r}), \quad (2.2)$$

where $\varepsilon(\mathbf{r})$ denotes the relative permittivity of the object and \mathbf{E}^m the macroscopic field inside the object, then we get

$$\nabla \times (\nabla \times \mathbf{E}^m(\mathbf{r})) = \varepsilon(\mathbf{r})k_0^2\mathbf{E}^m(\mathbf{r}), \quad (2.3)$$

with $k_0 = \omega^2/c^2$. Using the relationship $\varepsilon = \varepsilon_{\text{mul}} + 4\pi\chi$, where χ denotes the linear field susceptibility and ε_{mul} the relative permittivity of the multilayer system. Note that ε_{mul} depends only of z . Then, we have:

$$\nabla \times (\nabla \times \mathbf{E}^m(\mathbf{r})) - \varepsilon_{\text{mul}}k_0^2\mathbf{E}^m(\mathbf{r}) = 4\pi\chi(\mathbf{r})k_0^2\mathbf{E}^m(\mathbf{r}). \quad (2.4)$$

To solve this equation one needs the Green function defined as:

$$\nabla \times (\nabla \times \mathbf{G}(\mathbf{r}, \mathbf{r}')) - \varepsilon_{\text{mul}}k_0^2\mathbf{G}(\mathbf{r}, \mathbf{r}') = 4\pi k_0^2\mathbf{I}\delta(\mathbf{r} - \mathbf{r}'), \quad (2.5)$$

and the solution of Eq. (2.4) reads:

$$\mathbf{E}^{\text{m}}(\mathbf{r}) = \mathbf{E}_{\text{ref}}(\mathbf{r}) + \int_{\Omega} \mathbf{G}(\mathbf{r}, \mathbf{r}') \chi(\mathbf{r}') \mathbf{E}^{\text{m}}(\mathbf{r}') d\mathbf{r}', \quad (2.6)$$

where \mathbf{E}_{ref} is the field in the absence of the object and Ω the support of the object under study. When we solve Eq. (2.4) the field \mathbf{E}^{m} corresponds to the macroscopic field inside the object. To solve Eq. (2.4) we discretize the object in a set of N subunits with a cubic meshsize d , then the integral equation becomes the sum of N integrals:

$$\mathbf{E}^{\text{m}}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \int_{V_j} \mathbf{G}(\mathbf{r}_i, \mathbf{r}') \chi(\mathbf{r}') \mathbf{E}^{\text{m}}(\mathbf{r}') d\mathbf{r}', \quad (2.7)$$

with $V_j = d^3$. Assuming the field, the Green function and the susceptibility constant over a subunit we get:

$$\mathbf{E}^{\text{m}}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \mathbf{G}(\mathbf{r}_i, \mathbf{r}_j) \chi(\mathbf{r}_j) \mathbf{E}^{\text{m}}(\mathbf{r}_j) d^3. \quad (2.8)$$

We can share into two parts the Green function, $\mathbf{G} = \mathbf{M} + \mathbf{T}$, where \mathbf{M} is the Green function who take into account of the multiple reflection between the different layers and \mathbf{T} is the Green function of the homogeneous space. Using, in first approximation (the radiative reaction term neglected) $\int_{V_i} \mathbf{T}(\mathbf{r}_i, \mathbf{r}') d\mathbf{r}' = -4\pi/(3\varepsilon_{\text{mul}}(\mathbf{r}_i))$ ⁵, we get:

$$\mathbf{E}^{\text{m}}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \mathbf{G}'(\mathbf{r}_i, \mathbf{r}_j) \chi(\mathbf{r}_j) d^3 \mathbf{E}^{\text{m}}(\mathbf{r}_j) - \frac{4\pi}{3\varepsilon_{\text{mul}}(\mathbf{r}_i)} \chi(\mathbf{r}_i) \mathbf{E}^{\text{m}}(\mathbf{r}_i), \quad (2.9)$$

where $\mathbf{G}' = \mathbf{M} + \mathbf{T}$ for $i \neq j$ and $\mathbf{G}' = \mathbf{M}$ for $i = j$, then we can write

$$\mathbf{E}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \mathbf{G}'(\mathbf{r}_i, \mathbf{r}_j) \alpha_{\text{CM}}(\mathbf{r}_j) \mathbf{E}(\mathbf{r}_j) \quad (2.10)$$

$$\text{with } \mathbf{E}(\mathbf{r}_i) = \frac{\varepsilon(\mathbf{r}_i) + 2\varepsilon_{\text{mul}}(\mathbf{r}_i)}{3\varepsilon_{\text{mul}}(\mathbf{r}_i)} \mathbf{E}^{\text{m}}(\mathbf{r}_i) \quad (2.11)$$

$$\alpha_{\text{CM}}(\mathbf{r}_j) = \frac{3}{4\pi} \varepsilon_{\text{mul}}(\mathbf{r}_i) d^3 \frac{\varepsilon(\mathbf{r}_i) - \varepsilon_{\text{mul}}(\mathbf{r}_i)}{\varepsilon(\mathbf{r}_i) + 2\varepsilon_{\text{mul}}(\mathbf{r}_i)}. \quad (2.12)$$

The field $\mathbf{E}(\mathbf{r}_i)$ is the local field, *i.e.* the field at the position i in the absence of the subunit i . Then the linear system can be written formally as

$$\mathbf{E} = \mathbf{E}_{\text{ref}} + \mathbf{A} \mathbf{D}_{\alpha} \mathbf{E}, \quad (2.13)$$

where \mathbf{A} is a matrix which contains all the Green function and \mathbf{D}_{α} is a tridiagonal matrix with the polarizabilities of each element of discretization. In the next chapter we detail how to solve Eq. (2.13) rigorously, but in this present chapter we detail different approached methods to avoid the tedious resolution of Eq. (2.13). The scattered field is computed through

$$\mathbf{E}^{\text{d}}(\mathbf{r}) = \sum_{j=1}^N \mathbf{G}(\mathbf{r}, \mathbf{r}_j) \alpha(\mathbf{r}_j) \mathbf{E}(\mathbf{r}_j). \quad (2.14)$$

2.2 Approximated method

2.2.1 Born

The most simple approximation is the Born approximation which consists to assume the field inside the object equal to the reference field for each element of discretization:

$$\mathbf{E}^m(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i), \quad (2.15)$$

This approximation hold if the contrast is weak and the object small compare to the wavelength of illumination.

2.2.2 Renormalized Born

The renormalized Born approximation consists to assume the local field inside the object equal to the reference field :

$$\mathbf{E}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i). \quad (2.16)$$

In that case the macroscopic field reads:

$$\mathbf{E}^m(\mathbf{r}_i) = \frac{3\varepsilon_{\text{mul}}}{\varepsilon(\mathbf{r}_i) + 2\varepsilon_{\text{mul}}} \mathbf{E}_{\text{ref}}(\mathbf{r}_i). \quad (2.17)$$

This approximation is better that the classical Born approximation when the permittivity is high.

2.2.3 Born at the order 1

To be more precise that the renormalized Born approximation, one can perform the Born series at the order one:

$$\mathbf{E}(\mathbf{r}_i) = \mathbf{E}_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N \mathbf{G}'(\mathbf{r}_i, \mathbf{r}_j) \alpha(\mathbf{r}_j) \mathbf{E}_{\text{ref}}(\mathbf{r}_j). \quad (2.18)$$

In that case we take into account the simple scattering.

2.2.4 Scalar Approximation revisited

We only consider configurations where the reference field in Ω can be written as $\mathbf{E}_{\text{ref}}(\mathbf{r}) = E_{\text{ref}}(\mathbf{r})\mathbf{u}$ with \mathbf{u} a complex vector such that $\mathbf{u} \cdot \mathbf{u}^* = 1$ where $*$ stands for the complex conjugate and $E_{\text{ref}}(\mathbf{r})$ a complex function. This is the case if the reference field in Ω is a plane wave and the object is located in the superstrat.

In our approach, we assume that the field inside Ω is directed along \mathbf{u} so that $\mathbf{E}^m(\mathbf{r}) \approx E_u(\mathbf{r})\mathbf{u}$ where E_u is a complex function. In this case, taking the scalar product of Eq. (2.8) with \mathbf{u}^* yields an integral scalar equation for E_u ,

$$\begin{aligned} \mathbf{u}^* \cdot \mathbf{E}^m(\mathbf{r}) &= \mathbf{u}^* \cdot \mathbf{E}_{\text{ref}}(\mathbf{r})\mathbf{u}^* \cdot \int_{\Omega} \mathbf{G}(\mathbf{r}, \mathbf{r}') \chi(\mathbf{r}') E_u^m(\mathbf{r}') \mathbf{u} d\mathbf{r}' \\ E_u^m(\mathbf{r}) &= E_{\text{ref}}(\mathbf{r}) + \int_{\Omega} [\mathbf{u}^* \cdot \mathbf{G}(\mathbf{r}, \mathbf{r}')\mathbf{u}] \chi(\mathbf{r}') E_u^m(\mathbf{r}') d\mathbf{r}', \end{aligned} \quad (2.19)$$

where the green tensor has been replaced by the scalar function, $g_u(\mathbf{r}, \mathbf{r}') = \mathbf{u}^* \cdot \mathbf{G}(\mathbf{r}, \mathbf{r}') \mathbf{u}$. Then the field inside Ω is computed through:

$$E_u^{\text{m}}(\mathbf{r}_i) = E_{\text{ref}}(\mathbf{r}_i) + \sum_{j=1}^N g_u(\mathbf{r}_i, \mathbf{r}_j) \chi(\mathbf{r}_j) E_u^{\text{m}}(\mathbf{r}_j) d^3, \quad (2.20)$$

with $i = 1, \dots, N$. It is obvious that the size of the vector and the matrix are decreased by a factor 3. Then, when we solve iteratively the linear system, as it needs only to treat one component, we guess that the numerical computation will be faster by a factor 3 at least. Notice that once the near field is obtained, we transform it in vectorial form with $\mathbf{E}^{\text{m}}(\mathbf{r}_i) = E_u^{\text{m}}(\mathbf{r}_i) \mathbf{u}$ and we use it to obtain the far field.

2.3 Computation of the Green function

Even though we are using an efficient integration scheme to evaluate the Green tensor, see Ref. 6, it takes a lot of time to evaluate it for all the different pair of points covering the object. Note that due to the translational invariance of the reference medium in the (x, y) plane, $\mathbf{G}(\mathbf{r}, \mathbf{r}') = \mathbf{G}(\|\mathbf{r}_{\parallel} - \mathbf{r}'_{\parallel}\|, z, z')$. For each couple (z, z') , the number of pairs with different distances of a Cartesian (x, y) mesh with $n_x \times n_y$ points ($n_x > n_y$) is equal to $n_y(2n_x - n_y + 1)/2$. To accelerate the computation, we approximate $\mathbf{G}(\|\mathbf{r}_{\parallel} - \mathbf{r}'_{\parallel}\|, z, z')$ using an interpolation of a discrete set of points, $\mathbf{G}(qd/n_d, z, z')$ with $q = 1, \dots, \text{int} \sqrt{n_x^2 + n_y^2}$ and n_d a natural number. Linear and polynomial interpolations could not evaluate the Green tensor properly when $\|\mathbf{r}_{\parallel} - \mathbf{r}'_{\parallel}\| < \lambda$, as the fast decay of the evanescent waves was not accounted for accurately. We obtained much better results using rational functions, that is quotients of polynomials. Rational functions have the ability to model functions with poles (Press et al. 1986) and permit an accurate approximation of the $1/r^3$ behavior of the Green tensor in the near field range.

In the code, in the section numerical parameters, the drop menu Green function permits to choose to compute rigorously the Green function or evaluate the Green tensor with interpolation for $n_d = 1, 2, 3, 4$. Notice that by default the code uses $n_d = 2$ which is enough accurate. Note that only the computation with interpolation is parallelized.

Numerical details

Contents

3.1 Polarizability	9
3.2 Solve the system of linear equation	10
3.3 Change of the initial guess	11
3.4 Preconditioning the system of linear equations	11
3.5 The default options and how to change them	11

3.1 Polarizability

The DDA discretizes the object into a set of punctual dipoles, where a polarizability α is associated to each punctual dipoles. There are different forms for this polarizability. The first to have been used, and the simplest, is the relation of Clausius Mossotti (CM)²:

$$\alpha_{\text{CM}} = \frac{3}{4\pi} \varepsilon_{\text{mul}} \frac{\varepsilon - \varepsilon_{\text{mul}}}{\varepsilon + 2\varepsilon_{\text{mul}}} d^3 = \varepsilon_{\text{mul}} \frac{\varepsilon - \varepsilon_{\text{mul}}}{\varepsilon + 2\varepsilon_{\text{mul}}} a^3, \quad (3.1)$$

where ε denotes the permittivity of the object, d the size of the cubic meshsize and $a = \left(\frac{3}{4\pi}\right)^{\frac{1}{3}} d$ the radius of the sphere of the same volume than the cubic meshsize of the side d . Unfortunately, this relation does not keep the energy and, then, it is necessary to introduce a radiative reaction term that takes into account the fact that charges in movement lose energy, and the polarizability is, then, written as³:

$$\alpha_{\text{RR}} = \frac{\alpha_{\text{CM}}}{1 - \frac{2}{3} i k_0^3 n_{\text{mul}} \alpha_{\text{CM}}}. \quad (3.2)$$

After different forms of the polarizability have been established in order to improve the precision of the DDA and take into account the non-punctual character of the dipole, and we may quote, among the best known, the ones by Goedecke and O'Brien⁷,

$$\alpha_{\text{GB}} = \frac{\alpha_{\text{CM}}}{1 - \frac{2}{3} i k_0^3 n_{\text{mul}} \alpha_{\text{CM}} - k_0^2 \alpha_{\text{CM}} / a}, \quad (3.3)$$

by Lakhtakia⁸:

$$\alpha_{\text{LA}} = \frac{\alpha_{\text{CM}}}{1 - 2 \frac{\varepsilon - \varepsilon_{\text{mul}}}{\varepsilon + 2\varepsilon_{\text{mul}}} [(1 - i k_0 n_{\text{mul}} a) e^{i k_0 n_{\text{mul}} a} - 1]} \quad (3.4)$$

and Draine and Goodman⁹

$$\alpha_{\text{LR}} = \frac{\alpha_{\text{CM}}}{1 + \alpha_{\text{CM}} \left[\frac{(b_1 + \varepsilon b_2 / \varepsilon_{\text{mul}} + \varepsilon b_3 / \varepsilon_{\text{mul}} S) k_0^2}{d} - \frac{2}{3} i n_{\text{mul}} k_0^3 \right]}, \quad (3.5)$$

with $b_1 = -1.891531$, $b_2 = 0.1618469$, $b_3 = -1.7700004$ and $S = 1/5$.

Inside the code by default, it is α_{RR} which is used. In the case when the permittivity is anisotropic only α_{RR} is going to be used.

A last polarizability is introduced (PS) that only works for homogeneous spheres and is particularly precise for metals. This consists of making a change of the polarizability of the elements on the edge of the sphere taking into account the factor of depolarization of the sphere.¹⁰ Note that the sphere should be embedded in only one layer.

3.2 Solve the system of linear equation

In order to know the electric field in the object, *i.e.* the field at the position of the N elements of discretization, we have to solve the following system of linear equation:

$$\mathbf{E} = \mathbf{E}_0 + \mathbf{A} \mathbf{D}_\alpha \mathbf{E}, \quad (3.6)$$

where \mathbf{E}_0 is a vector of size $3N$ which contains the incident field at the discretization elements. \mathbf{A} is a matrix $3N \times 3N$ which contains all the field tensor susceptibility and \mathbf{D}_α is a diagonal matrix $3N \times 3N$, if the object is isotropic, or diagonal block 3×3 if the object is anisotropic. \mathbf{E} is the vector $3N$ which contains the unknown electric local fields. The equation is solved by a non-linear iterative method. The code proposes numerous iterative methods, and the one used by default is GPBICG because it is the most efficient in most cases¹¹. The code stops when the residue,

$$r = \frac{\|\mathbf{E} - \mathbf{A} \mathbf{D}_\alpha \mathbf{E} - \mathbf{E}_0\|}{\|\mathbf{E}_0\|}, \quad (3.7)$$

is under the tolerance given by the user. 10^{-4} is the tolerance used by default, because it is a good compromise between speed and precision. Please find below the different iterative method possible in the code:

- GPBICG1 : Ref. [12](#)
- GPBICG2 : Ref. [12](#)
- GPBICGsafe : Ref. [13](#)
- GPBICGAR1 : Ref. [12](#)
- GPBICGAR2 : Ref. [12](#)
- QMRCLA : Ref. [14](#)
- TFQMR : Ref. [14](#)
- CG : Ref. [14](#)
- BICGSTAB : Ref. [14](#)
- QMRBICGSTAB1 : Ref. [15](#)

- QMRBICGSTAB2 : Ref. 15
- GPBICOR : Ref. 16
- CORS : Ref. 17
- BiCGstar-plus Ref. 18

3.3 Change of the initial guess

When the system of linear equations is solved iteratively, we have the possibility to choose the starting point, *i.e.* the initial field \mathbf{E}_i to start the iterative method. The closer the solution chosen at the beginning will be close to the “good solution”, the more the number of iterations will be reduced. We therefore propose the possibility to choose as initial estimate for the field:

- $\mathbf{E}_i = \mathbf{0}$: null field at the beginning.
- $\mathbf{E}_i = \mathbf{E}_0$: Born approximation.
- Use of the scalar approximation $\mathbf{u.Gu}$. In this case, the scalar approximation is also solved iteratively but for $r = 0.01$. An additional precision would not be of interest, because we just want a correct starting point.

3.4 Preconditioning the system of linear equations

Another solution is to precondition the matrix to be inverted on the left to make the iterative method faster. That is to say instead of solving $(\mathbf{I} - \mathbf{A}\mathbf{D}_\alpha)\mathbf{E} = \mathbf{E}_0$, we must then solve $\mathbf{P}^{-1}(\mathbf{I} - \mathbf{A}\mathbf{D}_\alpha)\mathbf{E} = \mathbf{P}^{-1}\mathbf{E}_0$ where \mathbf{P} is a matrix close to $(\mathbf{I} - \mathbf{A}\mathbf{D}_\alpha)$ and whose inverse can be computed easily. For this matrix we have chosen a matrix of Chan¹⁹ on the two dimensions of space x and y ²⁰. This preconditioning is particularly efficient when the object under study is homogeneous or weakly inhomogeneous and has a small thickness in z compared to its dimensions in x and y . The preconditioning can also be done on the right side, *i.e.* we have to find \mathbf{X} such that $(\mathbf{I} - \mathbf{A}\mathbf{D}_\alpha)\mathbf{P}^{-1}\mathbf{X} = \mathbf{E}_0$, then deduce the field with $\mathbf{E} = \mathbf{P}^{-1}\mathbf{X}$.

Note that this preconditioning is also implemented for the scalar approximation.

3.5 The default options and how to change them

The default options chosen are:

- The polarizability: α_{RR} .
- The iterative method: GPBICG1.
- The tolerance of the iterative method: 10^{-4} .
- The maximum number of iterations of the iterative method: 1000
- The initial guess for the iterative method: Born approximation.
- The preconditioning: no preconditioning.
- Green’s function interpolation: level 2

All these options can be changed. To do this you must click on “Advanced interface”, and appears at the bottom a xcw hole section section called “Numerical parameters” where all the parameters related to the iterative method and the polarizability can be adapted.

Managing of the configurations

Contents

4.1	Introduction	13
4.2	Creation and saving of a new configuration	13
4.3	Managing of the configurations	13

4.1 Introduction

The Code is launched by `./cdm` inside the `bin` folder for a Linux configuration. It has been created to be as convenient as possible and so needing few explanations for its use. However, certain conventions have been taken and need to be clarified.

4.2 Creation and saving of a new configuration

In order to start a new calculation, go to the tab *calculation* and *New*. A new configuration shows up with values by default. Once the new configuration is chosen, in order to be saved, the tab *Calculation* and *Save* have to be selected again. Then, we select the name of the configuration, and we may add a short description of the calculation that has been made. Another way to save a configuration is to click directly on the panel of the configuration *Save configuration*. Then, two fields appear, one for the name of the configuration and the second one for its description.

4.3 Managing of the configurations

In order to manage all the selected configurations, we have go to the tab *Calculation* and *Load*. So, a new window appears with all the saved configurations. For each configuration there is a short description that the user has entered, the date, when the configuration file has been saved, then the principal characteristics of the configuration (wave length, power, the beam's waist, object, material, discretization and tolerance of the iterative method). It is enough to click on a configuration and to click on *load* in order to load a configuration.

The *delete* button is used to delete a saved configuration and the *export* enables to export inside a file (name of the configuration.opt) all the characteristics of the configuration.

Note that by double clicking on the line, we can modify the description field.

Properties of the illumination

Contents

5.1	Introduction	14
5.2	Beam	14
5.2.1	Introduction	14
5.2.2	Linear plane wave	15
5.2.3	Circular plane wave	16
5.2.4	Multiple plane wave	16
5.2.5	Linear Gaussian beam	16
5.2.6	Circular Gaussian	16
5.2.7	Speckle	17
5.2.8	Antenna	17
5.2.9	Arbitrary wave	18

5.1 Introduction

In the section properties of the illumination, the field *Wavelength* enables us to enter the using wavelength in vacuum. This one is entered in nanometer. The field *P₀* enables to enter the power of the laser beam in Watt. The field *W₀* in nanometer enables to enter for a plane wave the radius of the laser beam and for a Gaussian beam, the waist of the beam.

Note that the beam always propagates in the direction of the positive z axis, hence for $k_z > 0$ whatever the beam chosen.

5.2 Beam

5.2.1 Introduction

There are six beams predefined, their propagation direction is always defined in the same way, with two angles θ and φ , except for the speckle. They are connected to the given direction by the wave vector as follows:

$$k_x = k_0 \sin \theta \cos \varphi \quad (5.1)$$

$$k_y = k_0 \sin \theta \sin \varphi \quad (5.2)$$

$$k_z = k_0 \cos \theta \quad (5.3)$$

where $\mathbf{k}_0 = (k_x, k_y, k_z)$ is the wave vector parallel to the direction of the incident beam and k_0 the wave number, see Fig. 5.1. For the polarization, we use the plane (x, y) as

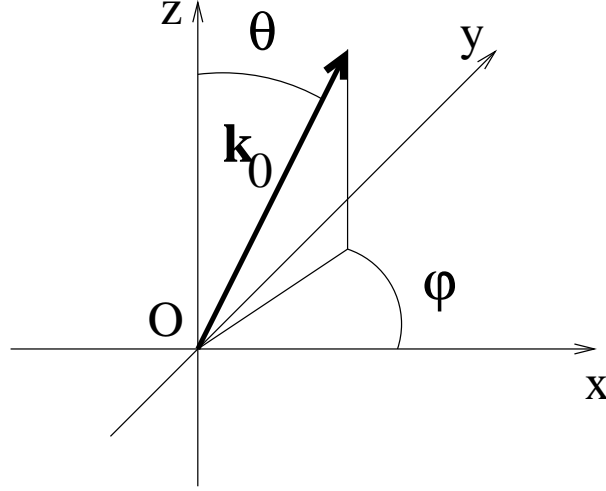


Figure 5.1 : *Definition of the beam's direction*

referential surface. Then, we can determine a polarization TM (p) and TE (s) with the presence of a surface, see Fig. 5.2 or a polarization along the x or y axis, depending on the beam. The frame (x, y, z) is used as an absolute referential. We define the polarization

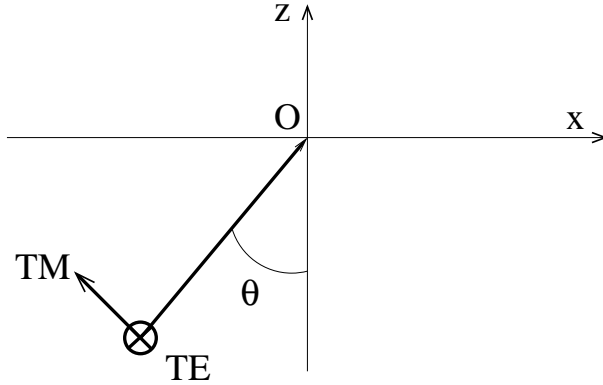


Figure 5.2 : *Definition of the beam's polarization.*

vector \mathbf{s} corresponding to TE polarisation and \mathbf{p} corresponding to TM as,

$$\mathbf{s} = \frac{\hat{\mathbf{z}} \times \mathbf{k}_0}{\|\hat{\mathbf{z}} \times \mathbf{k}_0\|} \quad (5.4)$$

$$\mathbf{p} = \frac{\mathbf{k}_0 \times \mathbf{s}}{\|\mathbf{k}_0 \times \mathbf{s}\|}. \quad (5.5)$$

5.2.2 Linear plane wave

Linear plane wave is a plane wave linearly polarized. The first line is relative to θ and the second to φ . The third line is connected to the polarization, polarization TM(1) or TE(0) as $\mathbf{E}_0 = E_p \mathbf{p} + E_s \mathbf{s}$ with $E_p = \text{pola}$ and $E_s = \sqrt{1 - \text{pola}^2}$. Note that the

polarization is not necessarily purely in TE or TM: $\text{pola} \in [0 \ 1]$ such as $E_{\text{TM}}^2 = \text{pola}^2 E^2$ and $E_{\text{TE}}^2 = (1 - \text{pola}^2) E^2$.

Notice that if one wants that $\mathbf{E}_0 \cdot \hat{\mathbf{x}} = 0$ ($\mathbf{E}_0 \cdot \hat{\mathbf{y}} = 0$), one can choose $\text{pola}=3$ (2) and the code will compute the right value of pola to get the polarization asked.

Note that the phase is always taken null at the origin of the frame, with Irradiance = P_0/S where $S = \pi w_0^2$ is the surface of the beam and $E_0 = \sqrt{2\text{Irradiance}/c/\varepsilon_0}$.

5.2.3 Circular plane wave

pwavircular is a plane wave circularly polarized. The first line is relative to θ and the second to φ . The third line is connected to the polarization that we can choose right (1) or left (-1) circular.

Note that the phase is taken null at the origin of the frame, with Irradiance = P_0/S where $S = \pi w_0^2$ is the surface of the beam and $E_0 = \sqrt{2\text{Irradiance}/c/\varepsilon_0}$.

5.2.4 Multiple plane wave

Multiple wave consists to take many planes waves. The first thing to do is to choose the number of plane wave, and then for each plane wave we choose θ and φ and the polarization. We have to write also the complex magnitude of each plane wave. The sum of the power of all the plane wave is equal to P_0 .

5.2.5 Linear Gaussian beam

Linear Gaussian is a Gaussian wave polarized linearly. The first line is relative to θ and the second to φ . The third line is connected to the angle between the polarization and the x axis (0) or along the y axis (90).

The three following lines help to fix the position of the centre (x_0, y_0, z_0) of the waist in nanometers in the frame (x, y, z) .

Note that this Gaussian beam may have a very weak waist, because it is calculated without any approximation through an angular spectrum representation done with FFT with always $k_z > 0$ whatever the inclination θ of the Beam. The definition of the waist, for a beam propagating along the z axis is :²¹

$$E(x, y, 0) = E_0 e^{-\rho^2/(2w_0^2)}, \quad (5.6)$$

with $\rho = \sqrt{x^2 + y^2}$. Then to compute a Gaussian beam polarized along the x axis, we have the magnitude of the Fourier component as:

$$\mathbf{A}(k_x, k_y) = E_0(k_z \mathbf{i} - k_x \mathbf{k}) \frac{1}{\sqrt{k_x^2 + k_z^2}} w_0 e^{-(k_x^2 + k_y^2)w_0^2/2}, \quad (5.7)$$

then we compute the reference field, $\mathbf{A}_{\text{ref}}(k_x, k_y, z)$, through the multilayer system, and the reference field reads:

$$\mathbf{E}_{\text{ref}}(x, y, z) = \int \int_{k_0} \mathbf{A}_{\text{ref}}(k_x, k_y, z) e^{i(k_x(x-x_0) + k_y(y-y_0) - k_z z_0)} d\mathbf{k}_{\parallel}. \quad (5.8)$$

5.2.6 Circular Gaussian

Circular Gaussian is a Gaussian wave circularly polarized. The first line is relative to θ and the second to φ . The third line is connected to the polarization that we can choose right (1) or left (-1) circular.

The next three lines enable us to fix the position of the centre of the waist in nanometers in the frame (x, y, z) .

Note that this Gaussian wave may have a very weak waist, because it is calculated without any approximation through a plane wave spectrum.

5.2.7 Speckle

Speckle is done as the Gaussian beam with a FFT but with a magnitude with a random phase. For a speckle polarized along the x axis the magnitude of the Fourier component is:

$$\mathbf{A}(k_x, k_y) = E_0(k_z \mathbf{i} - k_x \mathbf{k}) \frac{1}{\sqrt{k_x^2 + k_z^2}} e^{i\varphi}, \quad (5.9)$$

where φ is random variable between 0 and 2π . Then we compute the reference field, $\mathbf{A}_{\text{ref}}(k_x, k_y, z)$, through the multilayer system, and the reference field reads:

$$\mathbf{E}_{\text{ref}}(x, y, z) = \int \int_{k_0 \text{NA}} \mathbf{A}_{\text{ref}}(k_x, k_y, z) e^{i(k_x(x-x_0) + k_y(y-y_0) - k_z z_0)} d\mathbf{k}_{\parallel}, \quad (5.10)$$

where NA is the numerical aperture of the microscope. \mathbf{r}_0 permits to shift the speckle and the seed to change the distribution of the speckle.

5.2.8 Antenna

It is possible to illuminate the object with a dipolar antenna. For this illumination the orientation of the dipole must be given (θ angle between the dipole and the z axis, and φ angle that the projection of the dipole on the (x, y) plane done with the x axis) and its position in x , y and z .

The location of the dipole can be outside the object or inside the object. When the antenna is in the object, it is then placed at the position of an element of discretization, as close as possible to the position given by the user.

The power given in the code (P_0) then corresponds to the total power radiated by the antenna.

Note that the radiation of a dipole is such that there are many energy radiated on the edge of the numerical aperture of the microscope. It is therefore necessary to take many points in the numerical aperture if you want to be precise.

Moreover, we should pay attention as the conservation of energy it is not necessarily respected. Indeed, a dipole which emits 1 W in vacuum, will not emit 1 W when it is close to an object or an interface. For example for the configuration shown Fig. 5.3(a), the normalized power is a function of the distance from the antenna to the interface, see Fig. 5.3(b). The radiation of a dipole is not an intrinsic quantity but depends on its environment. If one traces the inverse of the total power radiated by the dipole, it is proportional to the lifetime of a fluorescent atom, see Fig. 5.3(c). For more details, please refer to the items [22,23](#), but we can see that when a dipole approaches an interface then its evanescent waves are passing in propagating waves which increases the total power radiated when the dipole is very close to the interface.

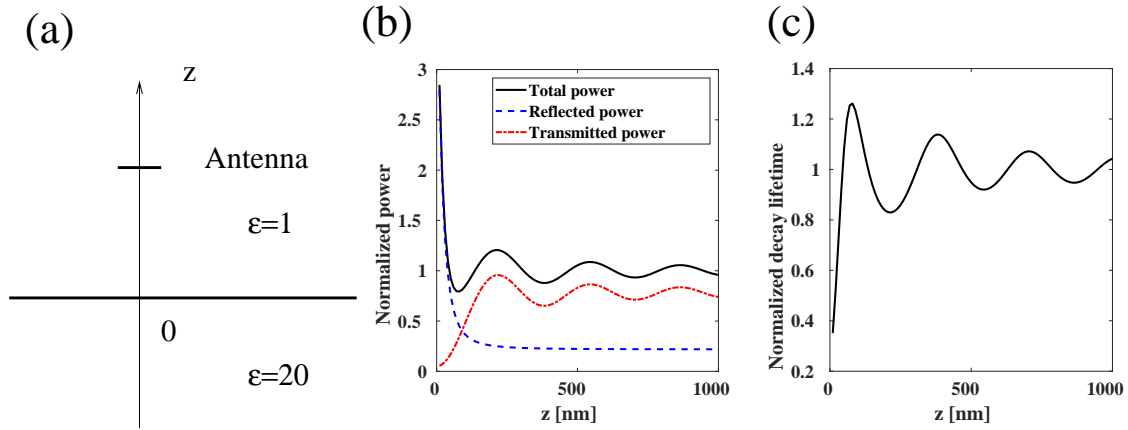


Figure 5.3 : (a) Configuration: Antenna in a vacuum above an interface of permittivity $\epsilon = 20$ (b) Total radiated power versus the distance from the antenna to the interface. (c) Lifetime of a fluorescent atom as a function of its distance from the interface.

5.2.9 Arbitrary wave

In the case of an arbitrary field, the characteristic are determined by the user. In other words, he has to create the field himself, and it is mandatory to create these files respecting the chosen conventions by the code.

The description of the discretization of the incident field is done within a file which is asked for when we click on *Props*. For example, for the real part of the component x of the field, it has to be constructed as follows:

```
nx,ny,nz
dx,dy,dz
xmin,ymin,zmin
```

- nx is the number of meshsize according to the axis x
- ny is the number of meshsize according to the axis y
- nz is the number of meshsize according to the axis z
- dx is the step according to the axis x
- dy is the step according to the axis y
- dz is the step according to the axis z
- xmin the smallest abscissa
- ymin the smallest ordinate
- zmin the smallest azimuth

Then, the files of the electric field are created as follows for each of the components of the real part and separated imaginary field:

```
open(11, file='Exr.mat', status='new', form='formatted', access='direct', recl=22)
do k=1,nz
```



```
do j=1,ny
  do i=1,nx
    ii=i+nx*(j-1)+nx*ny*(k-1)
    write(11,FMT='(D22.15)',rec=ii) dreal(Ex)
  enddo
enddo
enddo
```

Be careful, the mesh size of the discretization of the object has to be larger than the meshsize of the discretization of the field.

Properties of the multilayer

Contents

6.1 Introduction	20
6.2 Remarks	21

6.1 Introduction

In the section properties of the multilayer, you should first choose the number of interface. Note that you can not choose zero, as in that case the free space code is more efficient. Once the number n of interface is fixed click on *Props*. It appears a new window with n interfaces and $n + 1$ media. The first medium corresponds to the substrate, *i.e.* the medium through which the light comes. The permittivity of this medium is obviously transparent (no absorption). Then the position of the first interface in nanometer is asked followed by the second medium, etc. The sign $-$ is associated to the substrat and the sign $+$ to the superstrat, then ϵ_- and ϵ_+ for the permittivity, respectively.

An example is given in Fig. 6.1

The last medium corresponds to the superstrate.

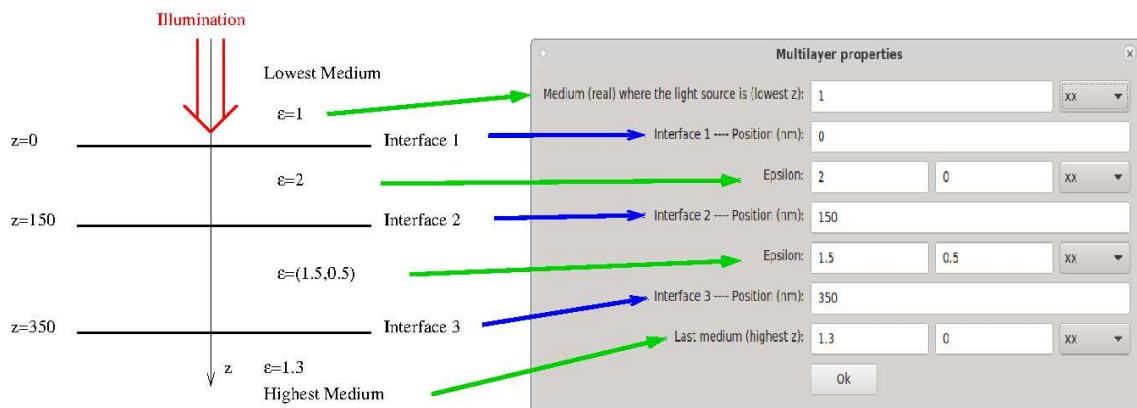


Figure 6.1 : How to configure the layer.

6.2 Remarks

- The last medium if one studies a microscope in transmission can not be absorbing.
- If the object under study contains one or more interfaces, note that any dipole (element of discretization) can be on a interface, then the code slightly moves the interface (less than one half mesh) to avoid this.
- The code is limited to 10 interfaces.
- Notice that if there is a large distance between two layers (several hundred of wavelength) the computation of the Green function can fail.
- The multilayer support guided mode resonance as the Green function is computed with the residue theorem.

Definition of the object

Contents

7.1	Introduction	22
7.2	Type of the object	22
7.2.1	Sphere	23
7.2.2	Inhomogeneous sphere	23
7.2.3	Cube	24
7.2.4	Cuboid (length)	24
7.2.5	Cuboid (meshsize)	24
7.2.6	Inhomogeneous Cuboid (length)	25
7.2.7	Inhomogeneous Cuboid (meshsize)	25
7.2.8	Ellipsoid	25
7.2.9	Multiple spheres	26
7.2.10	Cylinder	26
7.2.11	Concentric spheres	26
7.2.12	Arbitrary object	26
7.3	Choose the relative permittivity	27
7.4	Choose the discretization	28

7.1 Introduction

The code proposes several predefined objects, and we are going to precise in this section how to enter their optogeometrical characteristics. Note that all the distances have to be entered in nanometers. The code is doing the conversion in meters.

7.2 Type of the object

The list of the predefined objects is the following:

sphere, cube, cuboid, ellipsoid, cylinder, concentric spheres, multiple spheres, inhomogeneous sphere, inhomogeneous cuboid and arbitrary object.

When the objects as the cuboid, cylinder or ellipsoid have their edges turned with respect to the axes of the system of coordinates, the angles of Euler are used as defined

in Fig. 7.1. The rotation centre being the inertia centre of the object and the matrix of rotation reads:

$$\mathbf{A} = \begin{pmatrix} \cos(\psi) \cos(\varphi) - \sin(\psi) \cos(\theta) \sin(\varphi) & -\cos(\psi) \sin(\varphi) - \sin(\psi) \cos(\theta) \cos(\varphi) & \sin(\psi) \sin(\theta) \\ \sin(\psi) \cos(\varphi) + \cos(\psi) \cos(\theta) \sin(\varphi) & -\sin(\psi) \sin(\varphi) + \cos(\psi) \cos(\theta) \cos(\varphi) & -\cos(\psi) \sin(\theta) \\ \sin(\theta) \sin(\varphi) & \sin(\theta) \cos(\varphi) & \cos(\theta) \end{pmatrix}$$

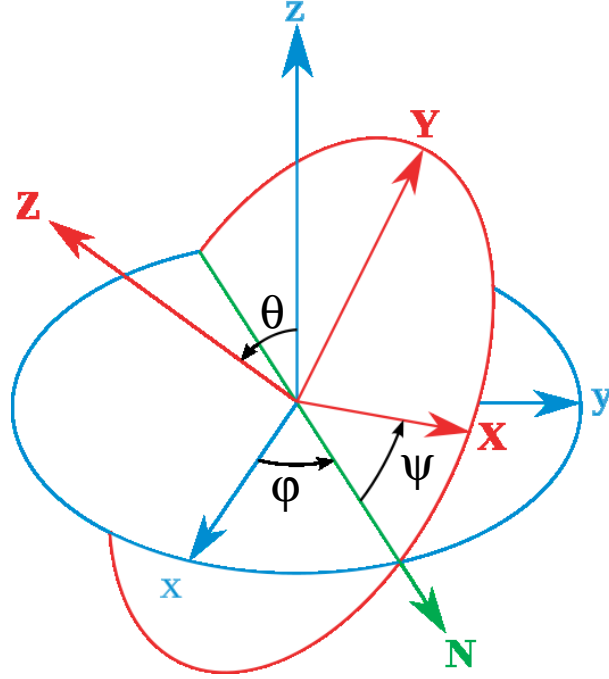


Figure 7.1 : Definition of the angles of Euler according to the convention $Z - X - Z$.
Scheme taken from Wikipedia

7.2.1 Sphere

For the sphere, there are four fields to be filled:

- The radius of the sphere in nanometer
- The abscissa of the centre of the sphere in nanometer
- The ordinate of the centre of the sphere in nanometer
- The azimuth of the centre of the sphere in nanometer

7.2.2 Inhomogeneous sphere

The permittivity of the sphere have a Gaussian noise with a correlation length l_c , standard deviation, A and an average ε_r .

For the inhomogeneous sphere there are seven fields to be filled:

- The radius of the sphere in nanometer
- The seed

- The abscissa of the centre of the sphere in nanometer
- The ordinate of the centre of the sphere in nanometer
- The azimuth of the centre of the sphere in nanometer
- The correlation length l_c
- The standard deviation A

7.2.3 Cube

For the cube, there are four fields to be filled:

- The edge of the cube in nanometer
- The abscissa of the centre of the sphere in nanometer
- The ordinate of the centre of the sphere in nanometer
- The azimuth of the centre of the sphere in nanometer

7.2.4 Cuboid (length)

For the cuboid, there are nine fields to be filled:

- The edge of the cube in nanometer according to the axis x
- The edge of the cube in nanometer according to the axis y
- The edge of the cube in nanometer according to the axis z
- The abscissa of the centre of the cuboid in nanometer
- The ordinate of the centre of the cuboid in nanometer
- The azimuth of the centre of the sphere in nanometer
- First angle of Euler ψ by rotation around the axis z
- Second angle of Euler θ by rotation around the axis x
- Third angle of Euler φ by rotation around the axis z

7.2.5 Cuboid (meshsize)

For the cuboid, there are seven fields to be filled:

- The abscissa of the centre of the cuboid in nanometer
- The ordinate of the centre of the cuboid in nanometer
- The azimuth of the centre of the sphere in nanometer
- Number of meshsize long x
- Number of meshsize long y
- Number of meshsize long z
- Meshsize in nanometer

7.2.6 Inhomogeneous Cuboid (length)

The permittivity of the cuboid have a Gaussian noise with a correlation length l_c , standard deviation A and an average ε_r . For the cuboid, there are nine fields to be filled:

- The edge of the cube in nanometer according to the axis x
- The edge of the cube in nanometer according to the axis y
- The edge of the cube in nanometer according to the axis z
- The abscissa of the centre of the cuboid in nanometer
- The ordinate of the centre of the cuboid in nanometer
- The azimuth of the centre of the sphere in nanometer
- The seed
- The correlation length l_c
- The standard deviation A

7.2.7 Inhomogeneous Cuboid (meshsize)

The permittivity of the cuboid have a Gaussian noise with a correlation length l_c , standard deviation A and an average ε_r . For the cuboid, there are nine fields to be filled:

- The abscissa of the centre of the cuboid in nanometer
- The ordinate of the centre of the cuboid in nanometer
- The azimuth of the centre of the sphere in nanometer
- Number of meshsize long x
- Number of meshsize long y
- Number of meshsize long z
- Meshsize in nanometer
- The seed
- The correlation length l_c
- The standard deviation A

7.2.8 Ellipsoid

For the ellipsoid, there are nine fields to be fulfilled:

- The half axis in nanometer according to the axis x
- The half axis in nanometer according to the axis y
- The half axis in nanometer according to the axis z
- The abscissa of the centre of the ellipse in nanometer

- The ordinate of the centre of the ellipse in nanometer
- The azimuth of the centre of the ellipse in nanometer
- First angle of Euler ψ by rotation around the axis z
- Second angle of Euler θ by rotation around the axis x
- Third angle of Euler φ by rotation around the axis z

7.2.9 Multiple spheres

For multiple spheres, it is convenient first to choose with the line from the under *number of objects* the number N of the expected spheres. Then, when we click on *Props N* windows, that we fill in the same way as for the unique sphere, appear. Beware, the spheres must be disconnected, otherwise, the code stops and shows error.

7.2.10 Cylinder

For the cylinder, there are eight fields to be fulfilled:

- The radius of the cylinder in nanometers
- The length of the cylinder in nanometer
- The abscissa of the centre of the cylinder in nanometer
- The ordinate of the centre of the cylinder in nanometer
- The azimuth of the centre of the cylinder in nanometer
- First angle of Euler ψ by rotation around the axis z
- Second angle of Euler θ by rotation around the axis x
- Third angle of Euler φ by rotation around the axis z

7.2.11 Concentric spheres

For concentric spheres, it is convenient first to choose with the under line *number of objects* the number N of concentric spheres. Then, when we click on *Props N* windows appear. The first window is filled the same way as for the sphere, and for the next windows, it is enough to enter the radius in nanometer. The radii must be entered in increasing order, otherwise, the code shows the error.

7.2.12 Arbitrary object

In the case of an arbitrary object, it is defined by the user. In other words, he has to create the object himself, and then, it is convenient to create this entry file by respecting the conventions chosen by the code. *namefile* is the name of the file containing the arbitrary object and it is asked for when we choose the arbitrary object. It is coded in sequential and in ascii, and is necessarily described inside a cuboid box. Below are given the lines of the code enabling to create this file:

```
open(15,file=namefile,status='old',iostat=ierror)
write(15,*) nx,ny,nz
```



```

write(15,*) aretecube
do i=1,nz
  do j=1,ny
    do k=1,nx
      write(15,*) xs(i,j,k),ys(i,j,k),zs(i,j,k)
    enddo
  enddo
enddo
do i=1,nz
  do j=1,ny
    do k=1,nx
      if objet isotrope
        write(15,*) eps(i,j,k)
      elseif objet anisotrope
        do ii=1,3
          do jj=1,3
            write(15,*) epsani(ii,jj,i,j,k)
          enddo
        enddo
      endif
    enddo
  enddo
enddo
enddo

```

- nx : size of the cuboid according to the axis x .
- ny : size of the cuboid according to the axis y .
- nz : size of the cuboid according to the axis z .
- aretecube : size of the meshsize of discretization in nanometers.
- x : abscissa of the mesh of discretization according the axis x .
- y : ordinate of the mesh of discretization according the axis y .
- z : azimuth of the mesh of discretization according the axis z .
- eps : epsilon of the object if isotropic
- epsani : epsilon of the object if anisotropic

7.3 Choose the relative permittivity

When the object or objects are chosen, it is then convenient to enter the relative permittivity. For the homogeneous object they may be isotropic or anisotropic. So, we choose *iso* or *aniso* and we click on *Epsilon*.

- *iso*: A board appears, where either we enter the relative permittivity by hand (real and imaginary part) or we choose a material in the data base.
- *aniso*: A board appears where we enter the relative permittivity by hand (real and imaginary part) for all the components of anisotropic tensor.

7.4 Choose the discretization

The number N_c entered in the field of the discretization corresponds to the number of layers forming the object in its largest direction.

A few examples:

- For an ellipse of half axis (a, b, c) , it is going to be the greatest half axis a that is going to be selected and the edge of discretization is going to be of $2a/N_c$.
- For a cube the number of meshsize is so going to be of $N = N_c^3$.

Possible study with the code

Contents

8.1	Introduction	29
8.2	Study in far field	29
8.3	Microscopy	31
8.4	Study in near field	32

8.1 Introduction

To determine the object with the appropriate orientation is not an easy task. That is why the first option *Only dipoles with epsilon*, enables us to check quickly if the object entered is well the one intended without any calculation being launched. Once this has been done, there are three great fields: the study in far field, the study in near field and the optical forces.

Important: Note that in the DDA the computation that takes the longest time is the calculation of the local field due to the necessity to solve the system of linear equations. One option has been added which consists in reading again the local field starting with a file. When this option is selected, the name of a file is asked for; either we enter an old file or a new name:

- If this is a new name, the calculation of the local field is going to be accomplished, then, stored together with the chosen configuration.
- If this is an old name, the local field is going to be read again with a checking that the configuration has not been changed between the writing and the second reading. This makes it easier to relaunch calculations very quickly for the same configuration but for different studies.

8.2 Study in far field

When the option far field is selected, three possibilities appear:

- *Cross section:* This option enables us to calculate the extinction (C_{ext}), absorbing (C_{abs}) and scattering cross section (C_{sca}). The scattering cross section is obtained

through $C_{\text{sca}} = C_{\text{ext}} - C_{\text{abs}}$. The extinction and absorption cross sections may be evaluated as:

$$C_{\text{ext}} = \frac{4\pi k_0}{\|\mathbf{E}_0\|^2} \sum_{j=1}^N \text{Im} [\mathbf{E}_0^*(\mathbf{r}_j) \cdot \mathbf{p}(\mathbf{r}_j)] \quad (8.1)$$

$$C_{\text{abs}} = \frac{4\pi k_0}{\|\mathbf{E}_0\|^2} \sum_{j=1}^N \left[\text{Im} [\mathbf{p}(\mathbf{r}_j) \cdot (\alpha^{-1}(\mathbf{r}_j))^* \mathbf{p}^*(\mathbf{r}_j)] - \frac{2}{3} k_0^3 \|\mathbf{p}^*(\mathbf{r}_j)\|^2 \right]. \quad (8.2)$$

Note that the cross section can only be computed if the background is homogeneous. The free space code is more adapted in that case, but it permits to check easily if the discretization is well adapted when a sphere is studied. Notice that the cross section can be computed if there is no interface.

- *Cross section+Poynting*: This option calculates also the scattering cross section from the integration of the far field diffracted by the object upon 4π steradians, the asymmetric factor when the background is homogeneous, else it computes only the differential cross section, *i.e.* $\langle \mathcal{P} \rangle = \langle \mathbf{S} \rangle \cdot \mathbf{n} R^2$ with \mathbf{S} the Poynting vector, \mathbf{n} the direction of observation, which is going to be represented in 3D. The values $N\theta$ and $N\phi$ enable us to give the number of points used in order to calculate the scattering cross and to represent the Poynting vector. The larger the object is, the larger $N\theta$ and $N\phi$ must be, which leads to time consuming calculations for objects of several wavelengths.

$$C_{\text{sca}} = \frac{k_0^4}{\|\mathbf{E}_0\|^2} \int \left\| \sum_{j=1}^N [\mathbf{p}(\mathbf{r}_j) - \mathbf{n}(\mathbf{n} \cdot \mathbf{p}(\mathbf{r}_j))] e^{-ik_0 \mathbf{n} \cdot \mathbf{r}_j} \right\|^2 d\Omega \quad (8.3)$$

$$g = \frac{k_0^3}{C_{\text{sca}} \|\mathbf{E}_0\|^2} \int \mathbf{n} \cdot \mathbf{k}_0 \left\| \sum_{j=1}^N [\mathbf{p}(\mathbf{r}_j) - \mathbf{n}(\mathbf{n} \cdot \mathbf{p}(\mathbf{r}_j))] e^{-ik_0 \mathbf{n} \cdot \mathbf{r}_j} \right\|^2 d\Omega \quad (8.4)$$

$$\frac{d \langle \mathcal{P} \rangle}{d\Omega} = \frac{1}{2} c \varepsilon_0 n \|\mathbf{E}_d(\mathbf{k}_{\parallel})\|^2, \quad (8.5)$$

where $\mathbf{E}_d(\mathbf{k}_{\parallel})$ is the diffracted field in far field.

A solution in order to go faster (option *quick computation*) and to pass by FFT for the calculation of the diffracted field. In this case, of course, it is convenient to discretize keeping in mind that the relation $\Delta x \Delta k = 2\pi/N$ connects the mesh size of the discretization with the size of the FFT. This is convenient for objects larger than the wavelength. Indeed, $L = N\Delta x$ corresponds to the size of the object which gives $\Delta k = 2\pi/L$, and if the size of the object is too small, then, the Δk is too large, and the quadrature is imprecise. Note that since the integration is performed on two planes parallel to the plane (x, y) , is not convenient if the incident makes an angle more than 70 degrees with the z axis. The 3D representation of the vector of Poynting is done as previously, *i.e.* with $N\theta$ and $N\phi$ starting with an interpolation upon the calculated points with the FFT.

- *Emissivity*. This study computes the reflectance, transmittance and absorptance. If the object under study is no absorbing then the absorptance should be zero. Then it traduces the level of energy conservation of our solver. It can depend of the precision of the iterative method and of the polarizability chosen.

8.3 Microscopy

This option permits to compute the image obtained for different microscope (holographic, brightfield, darkfield and phase). We consider a microscope made of an objective lens and a tube lens in $4f$ configuration and sine-Abbe condition²⁴ It asks for the numerical aperture of the objective lens ($NA = n_{\text{obj}} \sin \theta_{\text{obj}}$) and the numerical aperture of the condenser lens ($\sin \theta_{\text{cond}}$) for brightfield, darkfield and phase microscope. By default, the lenses are placed parallel to the plane (x, y) and their optical axis are confounded with the z axis. The focus plane of the lenses are placed to the origin of the frame but can be changed via the field “Position of the focal plane” for the microscope in transmission and reflection (Fig. 8.1). The magnification of the microscope is M and should be above 1. The drop menu propose three different microscope.

- *Holographic*: This option computes the diffracted field (Fourier plane) with the incident field defined in the section illumination properties. It computes the image plane with or without the presence of the incident field.
- *Brightfield*: This microscope uses a condenser lens, which focuses light from the light source onto the sample with a numerical aperture defined below the magnification. It consists to sum incoherently the image obtained with many incident field inside this numerical aperture with different polarization, hence it can take time as it needs to solve many direct problem. The result is given in the image plane without the incident field (a kind of dark field) and with the incident field (brightfield).
- *Darkfield & phase*: In darkfield microscopy the condenser is designed to form a hollow cone of light with a numerical aperture equal to the condenser lens, as apposed to brightfield microscopy that illuminates the sample with a full cone of light. The result is given in the image plane (scattered field). In the phase microscopy the ring-shaped illuminating light that passes the condenser annulus is focused on the specimen by the condenser exactly as in the dark field microscope and then the incident field with a phase shifted of $\pi/2$ is added to the scattered field.

The drop menu side computation permits to simulate microscope in transmission (Side $k_z > 0$), in reflection (Side $k_z < 0$), or both cases.

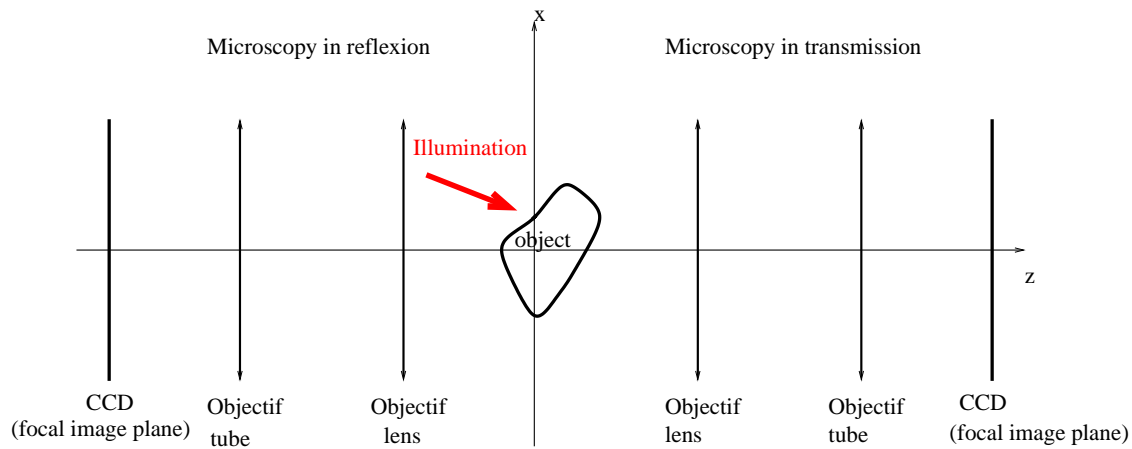


Figure 8.1 : Simplified figure of the microscope. The object focus of the objective lens are at the origin of the frame but can be changed. The axis of the lens is confounded with the z axis.

The calculation for the diffracted field may be completed starting with the sum of the radiation of the dipoles (very long when the object has a lot of dipoles) or with FFT (option *quick computation*) with a value $N = 128$ by default here as well. In this case, $\Delta x \Delta k = 2\pi/N$ with Δx the mesh size of discretization of the object which corresponds also to the discretization of the picture plane. Consequently, this one has a size of $L = GN\Delta x$.

The principle of the computation of the far field diffracted by the object and how to get the image through a microscope with a magnifying factor $M > 1$ has been detailed in Ref²⁵. Then we recall it briefly. The diffracted field in far field at a distance r of the origin in the direction (k_x, k_y) can be written as $\mathbf{E} = \mathbf{S}(k_x, k_y) \frac{e^{ikr}}{r}$. The field after the first lens (field in the Fourier space) is then defined as: $\mathbf{e}(k_{\parallel}) = \frac{\mathbf{S}(k_x, k_y)}{-2i\pi\gamma}$ with $\gamma = \sqrt{\epsilon_{\text{mul}}k_0^2 - k_x^2 - k_y^2}$ where the value of ϵ_{mul} corresponds to the permittivity of the substrate for the microscope in reflection and to the permittivity of the superstrate for the microscope in transmission. A microscope transforms a plane wave with wavevector \mathbf{k} into a plane wave with wavevector \mathbf{k}' with $\mathbf{k}' = [\mathbf{k}'_{\parallel}, \gamma']$ where $\mathbf{k}'_{\parallel} = (-k_x/M, -k_y/M)$ and $\gamma' = \sqrt{k_0^2 - k'_{\parallel}{}^2}$ (the refractive index in the image space is considered equal to 1). Then the field in the image space, after the tube lens, reads as:

$$\mathbf{E}_{\text{ob}}(\mathbf{r}) = \frac{1}{M} \iint \sqrt{\frac{\gamma}{\gamma'}} \tilde{h}(\mathbf{k}_{\parallel}) \mathbf{e}'(\mathbf{k}_{\parallel}) \exp[i\mathbf{k}' \cdot (\mathbf{r} - \mathbf{r}_f)] d\mathbf{k}_{\parallel}, \quad (8.6)$$

where $\tilde{h}(\mathbf{k}_{\parallel})$ is cutoff function allowing the transmission of only the signal included in the numerical aperture (NA) of the objective lens, it reads $\tilde{h}(\mathbf{k}_{\parallel}) = 1$ for $|\mathbf{k}_{\parallel}| < k_0 NA$ and 0 elsewhere and \mathbf{r}_f the position of the lens. We have

$$\mathbf{e}'(\mathbf{k}_{\parallel}) = \mathbf{R}(\mathbf{k}_{\parallel}) \mathbf{e}(\mathbf{k}_{\parallel}), \quad (8.7)$$

and $\mathbf{R}(\mathbf{k}_{\parallel})$ is given by:

$$\mathbf{R}(\mathbf{k}_{\parallel}) = \begin{pmatrix} u_x^2(1 - \cos \theta) + \cos \theta & u_x u_y(1 - \cos \theta) & u_y \sin \theta \\ u_x u_y(1 - \cos \theta) & u_y^2(1 - \cos \theta) + \cos \theta & -u_x \sin \theta \\ -u_y \sin \theta & u_x \sin \theta & \cos \theta \end{pmatrix}, \quad (8.8)$$

where $\mathbf{u} = \frac{\hat{\mathbf{k}} \times \mathbf{z}}{|\hat{\mathbf{k}} \times \mathbf{z}|}$ is the rotation axis. Notice that \mathbf{u} has no component along the z direction. θ is defined as $\cos \theta = \hat{\mathbf{k}} \cdot \hat{\mathbf{k}}'$ and $\sin \theta = \|\hat{\mathbf{k}} \times \hat{\mathbf{k}}'\|$

8.4 Study in near field

When the option near field is selected, two possibilities appear:

- *Local field*: This option enables us to draw the local field to the position of each element of discretization. The local field being the field at the position of each element of discretization in absence of itself.
- *Macroscopic field*: This option enables us to draw the macroscopic field to the position of each element of discretization. The connection between the local field and the macroscopic field is given Ref.⁴:

$$\mathbf{E}_{\text{macro}} = 3\epsilon_{\text{mul}} \left(\epsilon + 2\epsilon_{\text{mul}} - i \frac{k_0^3 d^3 \epsilon_{\text{mul}}^{3/2}}{2\pi} (\epsilon - \epsilon_{\text{mul}}) \right)^{-1} \mathbf{E}_{\text{local}} \quad (8.9)$$

The last option enables us to choose the mesh in which the local and macroscopic fields are represented.

- *Object*: Only the field in the object is represented. Notice that when FFT is used for the beam or for the computation of the diffracted field then this options is passed in the option *Cube*. This is same for the computation of the emissivity, the reread option and the use of the BPM(R).
- *Cube*: The field is represented within a cuboid containing the object.
- *Wide field*: The field is represented within a box greater than the object. The size of the box correspond to the size of the object plus the Additional side band (x , y or z) on each side. For example for a sphere with a radius $r = 100$ nm and discretization of 10, *i.e.* a meshsize of 10 nm, with an Additional side band x of 2, 3 for y and 4 for z , we get a box of size:

$$l_x = 100 + 2 \times 2 \times 10 = 140 \text{ nm} \quad (8.10)$$

$$l_y = 100 + 2 \times 3 \times 10 = 160 \text{ nm} \quad (8.11)$$

$$l_z = 100 + 2 \times 4 \times 10 = 180 \text{ nm} \quad (8.12)$$

The field inside the wide field area in near field is computed with

$$\mathbf{E} = \mathbf{E}_0 + \mathbf{ADE}, \quad (8.13)$$

which gives the field inside the near field zone and in the object.

Representation of the results

Contents

9.1 Introduction	34
9.2 Digital exits	34
9.3 Graphics	35
9.3.1 Plot epsilon/dipoles	35
9.3.2 Far field and microscopy	35
9.3.3 Study of the near field	36

9.1 Introduction

Three windows enable us to manage and represent the requested results. The one on the top enables us to manage the different figures; the one at the bottom on the left present the digital values requested, and the one at the bottom on the right is kept for the graphic representations.

9.2 Digital exits

All the results are given in the SI system.

- *Object subunits*: Number of elements of discretization of the object under study.
- *Mesh subunits* : Number of elements of discretization of the cuboid containing the object under study.
- *Mesh size* : Size of the element of discretization.
- $\lambda/(10|n|)$: In order to obtain a good precision, it is advised to have a discretization under the value of $\lambda/10$ in the considered material of optical index n .
- k_0 :Wave number.
- *Irradiance*: Beam irradiance, for a Gaussian beam, it is estimated at the center of the waist.
- *Field modulus*: Modulus of the field, for a Gaussian beam, it is estimated at the center of the waist.

- *Tolerance obtained*: Tolerance obtained for the chosen iterative method. Logically under the requested value.
- *Number of products Ax (iterations)*: Number of matrix vector products completed by the iterative method. Between brackets the iteration number of the iterative method.
- *Absorptivity* Fraction of radiation absorbed in %, equal to zero if all the permittivity are real.
- *Reflectivity* Fraction of radiation reflected in %.
- *Transmittivity* Fraction of radiation transmitted in %.
- *Extinction cross section*: Value of the extinction cross section.
- *Absorbing cross section*: Value of the absorbing cross section.
- *Scattering cross section*: Value of the scattering cross section obtained by = extinction cross section- absorbing cross section.
- *Scattering cross section with integration*: Value of the scattering cross section obtained by integration of the far field field radiated by the object.
- *Scattering asymmetric parameter*: Asymmetric factor.

9.3 Graphics

9.3.1 Plot epsilon/dipoles

The button *Plot epsilon/dipoles* enables us to see the position of each element of discretization. The colour of each point is associated with the value of the permittivity of the considered meshsize.

9.3.2 Far field and microscopy

9.3.2.1 Plot Poynting vector

Plot Poynting: enables us to draw the modulus of the Poynting vector in 3D. If the option quick computation is taken, then the results come from a interpolation of the points in the (k_x, k_y) space: if it is not smooth increase the number of point of the FFT.

9.3.2.2 Plot microscopy

Plot microscopy : enables us to draw the diffracted field in the Fourier plane for holographic microscope or the image through the dark field, brightfield, phase or holographic microscope. We can plot the modulus, intensity or the component x , y or z .

We have 8 different plot:

- *Fourier plane: Scattered field: $k_z > 0$* The diffracted field by the object in the Fourier plane for a holographic microscope in transmission.
- *Fourier plane: Total field: $k_z > 0$* The diffracted field by the object plus the incident field (if the incident field is a plane wave, then we have a Dirac) in the Fourier plane for a holographic microscope in transmission.

- *Fourier plane: Scattered field: $k_z < 0$* The diffracted field by the object in the Fourier plane for a holographic microscope in reflection.
- *Fourier plane: Total field: $k_z < 0$* The diffracted field by the object plus the incident field reflected on the multilayer system (if the incident field is a plane wave, then we have a Dirac) in the Fourier plane for a holographic microscope in reflection.
- *Image plane: Scattered field: $z > 0$* Image of the diffracted field by the object through the microscope in transmission.
- *Image plane: Total field: $z > 0$* Image of the diffracted field by the object plus the incident field through the microscope in transmission.
- *Image plane: Scattered field: $z < 0$* Image of the diffracted field by the object through the microscope in reflection.
- *Image plane: Total field: $z < 0$* Image of the diffracted field by the object plus the incident field through the microscope in reflection.

Remarks

- The diffracted field is represented upon a regular mesh in $\Delta k_x = \Delta k_y$ such as $\sqrt{k_x^2 + k_y^2} \leq k_0$ NA. If the computation is done by radiation of the dipoles, then the code choose to have at least 21 points in the numerical aperture. If quick computation is chosen then the code used FFT transform, then, the size of the picture is fixed by discretization of the object d with the relation $d\Delta k = 2\pi/N$ and N the size of the FFT.
- The computation in the image plane is always done with FFT.
- For the brightfield, darkfield and phase microscope only the field in the image plane can be plotted. When the option x , y and z component is chosen, the phase can not be plotted as we sum incoherently all the incidences, then we get only the modulus.

9.3.3 Study of the near field

- The first button *Field* enables us to choose to represent the incident field, local field or macroscopic field.
- The button *Type* enables us to represent the modulus or the component x , y or z of the studied field.
- The button *Cross section x (y or z)* enables us to choose the abscissa of the cut (ordinate or dimension). *Plot x (y or z)* draws the cut in plane x . *Plot all x* draws all the cut at once.

Output files for matlab, octave, scilab,...

Contents

10.1 Introduction	37
10.2 List of all exit files	38

10.1 Introduction

It is not necessary to use the graphic interface of the program to watch the results. For the scalar, all the results are in the output file and for the pictures, it is possible to use directly the exit files in ascii or in one hdf5 file and to read them through other software such as Matlab, Octave, Scilab,...For example in the directory bin the field ifdda.m uses matlab to represent the different data.

When the advanced option is chosen, it is possible to choose to save the data either in separate .mat files or in a single hdf5 file.

- In the case of the hdf5 file, there are six created groups: option (the options chosen by the user), near field (the near field data), microscopy (data from the microscopy), far field (data from the far field option), and dipole (position of the elements of discretization and permittivity).
- In the case of .mat file, all the output are formatted in the form of a unique column vector or two column vectors if the number is a complex (the real part being associated with the first column and the imaginary part with the second column).
- In the hdf5 file all the data are formatted under the form of a single column vector and with two separate tables in the case of complex numbers.
- In the case where the file contains three-dimensional data, these ones are always stored as follows:

```
do i=1,nz
  do j=1,ny
    do k=1,nx
      write(*,*) data(i,j,k)
```

```

    enddo
  enddo
enddo

```

Three-dimensional data are going to be recognized by 3D at the beginning of the line.

10.2 List of all exit files

All the files have the extension .mat if you choose the output in ascii file.

- x,y,z represent the different used coordinates.
- (3D) epsilon contain the permittivity of the object.
- (3D) xc,yc,zc contain the coordinates of all the points of the mesh.
- (3D) xwf,ywf,zwf contain the coordinates of all the points of the mesh in which the near field is calculated when the wide field option (wide field) is used.
- (3D complexe) incidentfieldx (y,z) contains the component $x(y,z)$ of the incidental field only inside the object.
- (3D) incidentfield contains the modulus of the incident field only inside the object.
- (3D complexe) macroscopicfieldx (y,z) contains the component $x(y,z)$ of the macroscopic field only inside the object.
- (3D) contains the modulus of the macroscopic field only inside the object.
- (3D complexe) localfieldx (y,z) contains the component $x(y,z)$ of the local field only inside the object.
- (3D) localfield contains the modulus of the local field only inside the object.
- (3D complexe) incidentfieldxwf (y,z) contains the component $x(y,z)$ of the incident field inside the box of near field in wide field.
- (3D) incidentfieldwf contains the modulus of the incidental field inside the box of near field in wide field.
- (3D complexe) macroscopicfieldxwf (y,z) contains the component $x(y,z)$ of the macroscopic field inside the box of near field in wide field.
- (3D) macroscopicfieldwf contains the modulus of the macroscopic field inside the box of near field in wide field.
- (3D complexe) localfieldxwf (y,z) contains the component $x(y,z)$ of the local field inside the box of near field in wide field.
- (3D) localfieldwf contains the modulus of the local field inside the box of near field in wide field.
- theta is a board which contains all the theta angles corresponding to all the directions in which the vector of Poynting is calculated. Its size is $(N_{\theta}+1)*N_{\phi}$.

- phi is a board which contains all the theta angles corresponding to all the directions in which the vector of Poynting is calculated. Its size is $(N_{\theta}+1)*N_{\phi}$.
- (2D) poynting contains the modulus of the vector of Poynting in theta and phi direction of size $(N_{\theta}+1)*N_{\phi}$.
- (2D) poyntingneg and poyntingpos contain the Poynting modulus for $k_z < 0$ and $k_z > 0$ respectively in the plane (k_x, k_y) .
- kx and ky contain the coordinates for poyntingneg and poyntingpos.
- (2D) fourierpos(x,y,z) contains the diffracted field in the fourier plane in modulus (x,y,z) for $k_z > 0$.
- (2D) fourierposinc(x,y,z) contains the total field in the fourier plane in modulus (x,y,z) for $k_z > 0$.
- (2D) fourierneg(x,y,z) contains the diffracted field in the fourier plane in modulus (x,y,z) for $k_z < 0$.
- (2D) fourierneginc(x,y,z) contains the total field in the fourier plane in modulus (x,y,z) for $k_z < 0$.
- kxfourier (kyfourier) contains the abscissa (ordinate) of the Fourier plane.
- (2D) imagepos(x,y,z) contains the diffracted field in the image plane in modulus (x,y,z) for $z > 0$.
- (2D) imageposinc(x,y,z) contains the total field in the image plane in modulus (x,y,z) for $z > 0$.
- (2D) imageneg(x,y,z) contains the diffracted field in the image plane in modulus (x,y,z) for $z < 0$.
- (2D) imageneginc(x,y,z) contains the total field in the image plane in modulus (x,y,z) for $z < 0$.
- (2D) imagebfpos(x,y,z) contains the diffracted field in the image plane in modulus (x,y,z) for a dark field with illumination inside the numerical aperture of the condenser for $z > 0$.
- (2D) imageincbfpos(x,y,z) contains the total field in the image plane in modulus (x,y,z) for a brightfield microscope for $z > 0$.
- (2D) imagebfneg(x,y,z) contains the diffracted field in the image plane in modulus (x,y,z) for a dark field with illumination inside the numerical aperture of the condenser for $z < 0$.
- (2D) imageincbfneg(x,y,z) contains the total field in the image plane in modulus (x,y,z) for a brightfield microscope for $z < 0$.
- (2D) imagedfpos(x,y,z) contains the diffracted field in the image plane in modulus (x,y,z) for a dark field with illumination with a hollow cone of light with a numerical aperture equal to the condenser lens for $z > 0$.
- (2D) imageincdfpos(x,y,z) contains field in the image plane in modulus (x,y,z) for a phase microscope for $z > 0$.

- (2D) `imagedfneg(x,y,z)` contains the diffracted field in the image plane in modulus (x,y,z) for a dark field with illumination with a hollow cone of light with a numerical aperture equal to the condenser lens for $z < 0$.
- (2D) `imageincdfneg(x,y,z)` contains field in the image plane in modulus (x,y,z) for a phase microscope for $z < 0$.
- (2D) `Ediffkposx (y,z)` contains the diffracted field by the object for $k_z > 0$ in the (k_x, k_y) plane.
- (2D) `Ediffknegx (y,z)` contains the diffracted field by the object for $k_z < 0$ in the (k_x, k_y) plane.
- `ximage` contains the x position for the images of microscopy.
- `yimage` contains the y position for the images of microscopy.
- `kxincident(bf)` and `(df)` plots the position of the component x of the incident wave vector for the bf (df) microscope.
- `kyincident(bf)` and `(df)` plots the position of the component y of the incident wave vector for the bf (df) microscope.

Some examples

Contents

11.1 Introduction	41
11.2 Test1	41
11.3 Test2	45
11.4 Test3	49
11.5 Test4	51

11.1 Introduction

In bin/tests there is the file options.db3. You should copy it in the directory bin as "cp options.db3.. /.', and then you launch the code after the load is appear four test configurations that allow you to see all the options in action.

11.2 Test1

The aim of test1 is to test a simple case and many options of the code to validate them. Figure [11.1](#) shows the options of the chosen configuration.

Start calculation

Save configuration

Calculation options

Rigorous

Read local field from file

Database file

Save in HDF5 file

Name h5 file

ifdda.h5

Advanced interface

Wavelength (nm)

632.8

P0 (W)

1

W0 (nm)

6328

Beam

Linear plane wave

Props

Number of plane waves

1

+

-

Number of interfaces

1

+

-

Props

Object

sphere

Props

Number of objects

1

+

-

Anisotropy

iso

Epsilon

Discretization

20

Only dipoles

Far field

Cross section:

Cross section + Poynting:

Ntheta:

72

Nphi:

144

Emissivity:

Microscopy

Type of Microscope:

Holographic

Quick computation (FFT):

Magnification factor:

100

Side Computation:

Both side

Numerical aperture: [0 n_f] (reflexion):

1.3

Position focal plane reflexion (nm):

0

Numerical aperture: [0 n_t] (transmission):

0.9

Position focal plane transmission (nm):

0

Near field

Local field:

Macroscopic field:

Range of study:

Wide field

Additional sideband x:

2

Additional sideband y:

3

Additional sideband z:

4

Tolerance

1e-09

Methode

GPBICG1

Green functions

Level 2

Polarizability


RR

FFT

1024

Figure 11.1 : Test1: configuration taken.

The following figures show the results obtained. The plots are done with Matlab and these are directly the eps files from the ifdda.m script that are used. The advantage of matlab in this case is to give all the figures in one go.

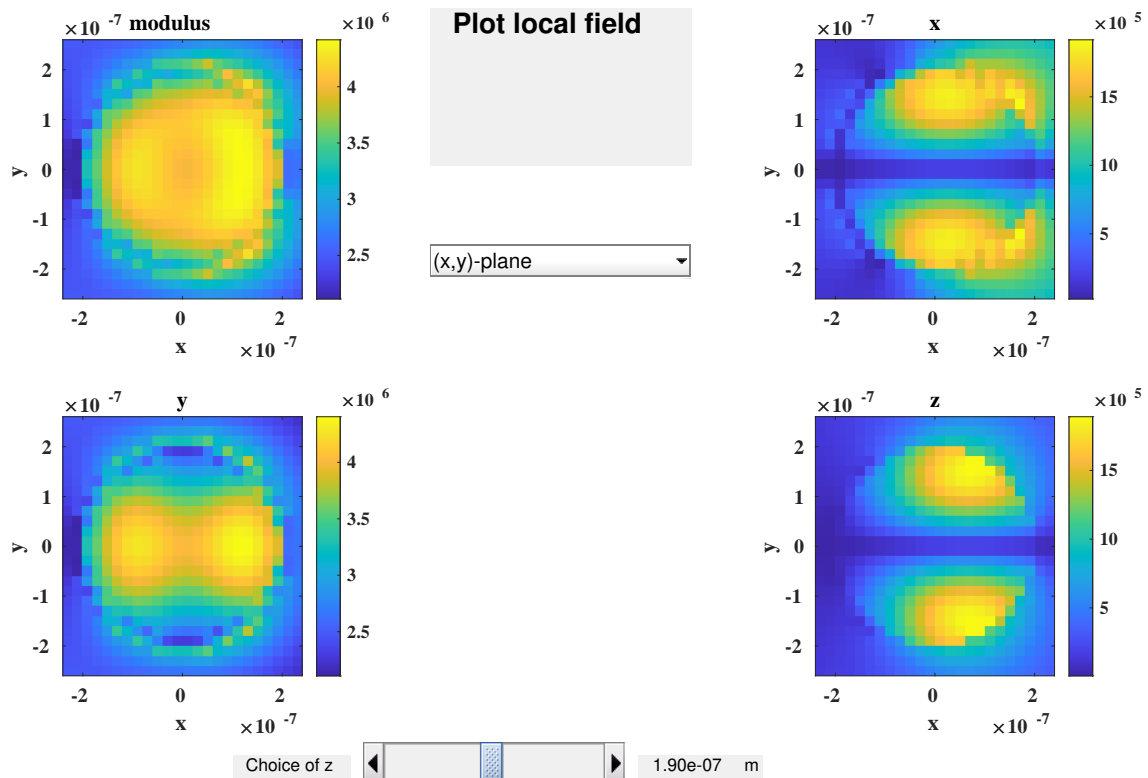Figure 11.2 : Modulus of the local field in (x,y) plane.

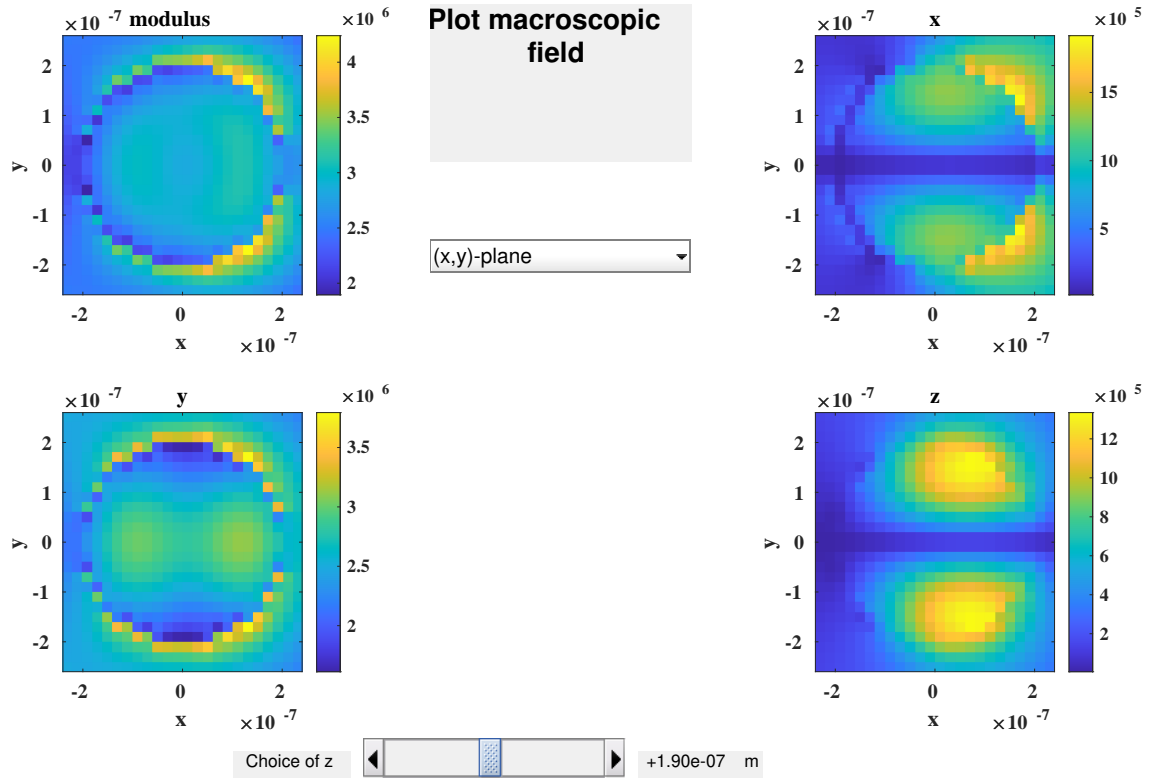


Figure 11.3 : Modulus of the macroscopic field in (x, y) plane.

Because the incident field is polarized along the y direction (TE), hence the y component of the field inside the sphere is the largest.

Poynting Modulus in k_x and k_y plane

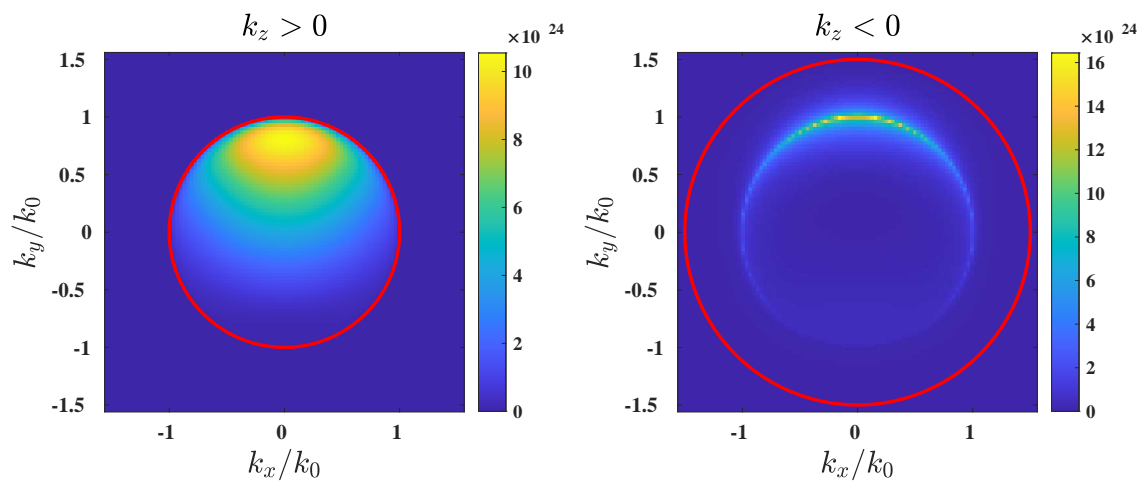


Figure 11.4 : Modulus of the Poynting vector.

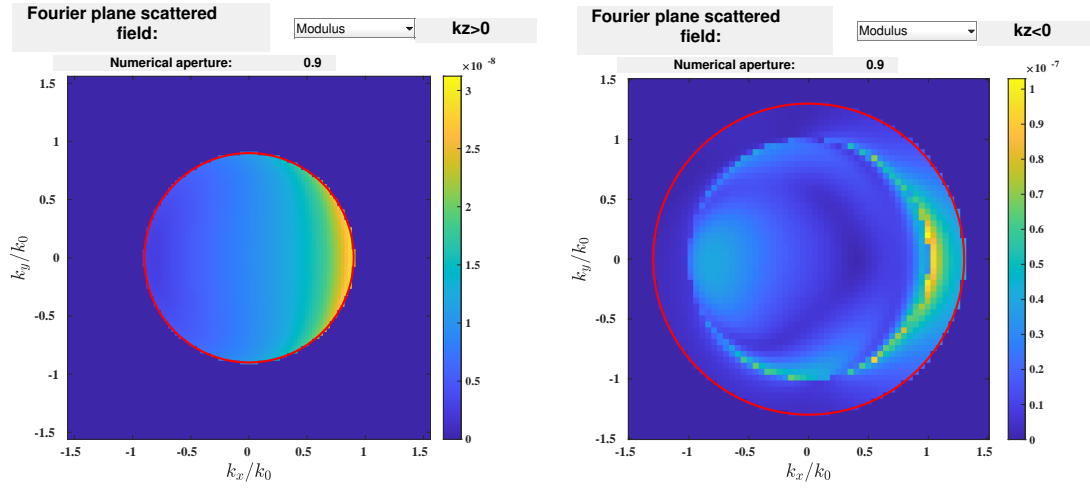


Figure 11.5 : Modulus of the diffracted field in the Fourier plane in transmission (left) and in reflection (right) for optical diffraction microscope.

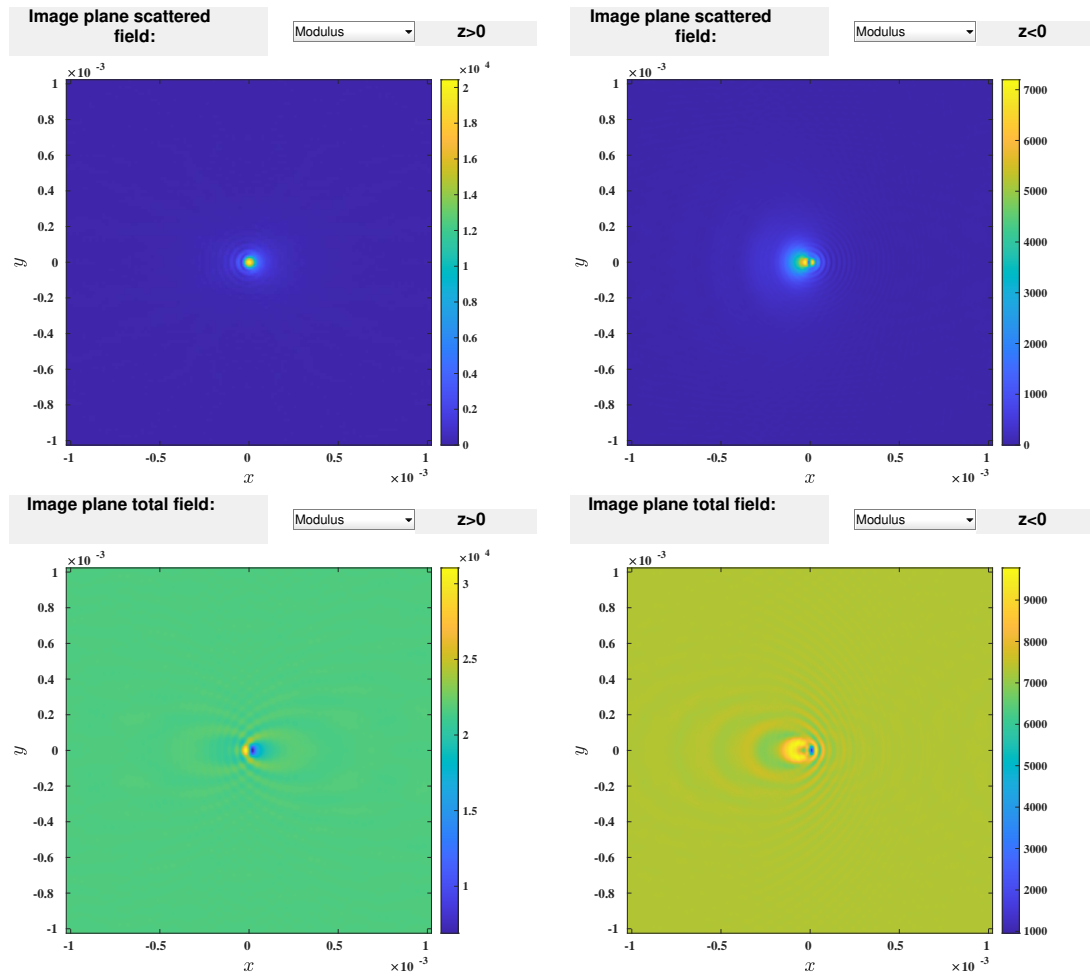


Figure 11.6 : Modulus of the field in the image plane in transmission (left) and in reflection (right) for optical diffraction tomography. Diffracted field (above) and total field (below).

11.3 Test2

The aim of the test2 is to test a more complex case. Figure 11.7 shows the options of the chosen configuration. The illumination is done with a Gaussian beam with $w_0 = \lambda$ and the object under study is a sphere with a radius of 500 nm and an inhomogeneous permittivity ($l_c = 100$ nm and $\sigma = 0.1$).

The screenshot displays the configuration interface for the Test2 simulation, organized into several panels:

- Top Left Panel:**
 - Buttons: "Start calculation" (red), "Save configuration"
 - Calculation options: "Rigorous" (dropdown)
 - Read local field from file: ☐
 - Database file: "Save in HDF5 file" (dropdown)
 - Name h5 file: "ifdda.h5" (text input)
 - Advanced interface: ☒
- Illumination properties:**
 - Wavelength (nm): 632.8
 - P0 (W): 1
 - W0 (nm): 632
 - Beam: "Linear Gaussian" (dropdown), "Props" button
 - Number of plane waves: 1 (with +/- buttons)
- Multilayer properties:**
 - Number of interfaces: 2 (with +/- buttons), "Props" button
- Object properties:**
 - Object: "inhomogeneous sphere" (dropdown), "Props" button
 - Number of objects: 1 (with +/- buttons)
 - Anisotropy: "iso" (dropdown), "Epsilon" button
 - Discretization: 40
- Study Panel:**
 - Only dipoles:** ☐
 - Far field:** ☒
 - Cross section: ☐
 - Cross section + Poynting: ☒
 - Ntheta: 36
 - Nphi: 72
 - Emissivity: ☒
 - Microscopy:** ☒
 - Type of Microscope: "Holographic" (dropdown)
 - Quick computation (FFT): ☒
 - Magnification factor: 100
 - Side Computation: "Both side" (dropdown)
 - Numerical aperture: [0 n_L] (reflexion): 1.3
 - Position focal plane reflexion (nm): 0
 - Numerical aperture: [0 n_L] (transmission): 0.9
 - Position focal plane transmission (nm): 0
 - Near field:** ☒
 - Local field: ☒
 - Macroscopic field: ☒
 - Range of study: "Cube around object" (dropdown)
- Numerical parameters Panel:**
 - Tolerance: 0.0001
 - Methode: "GPBICG1" (dropdown)
 - Green functions: "Level 2" (dropdown)
 - Polarizability: "RR" (dropdown)
 - FFT: 512 (dropdown)

Figure 11.7 : Test2: configuration taken.

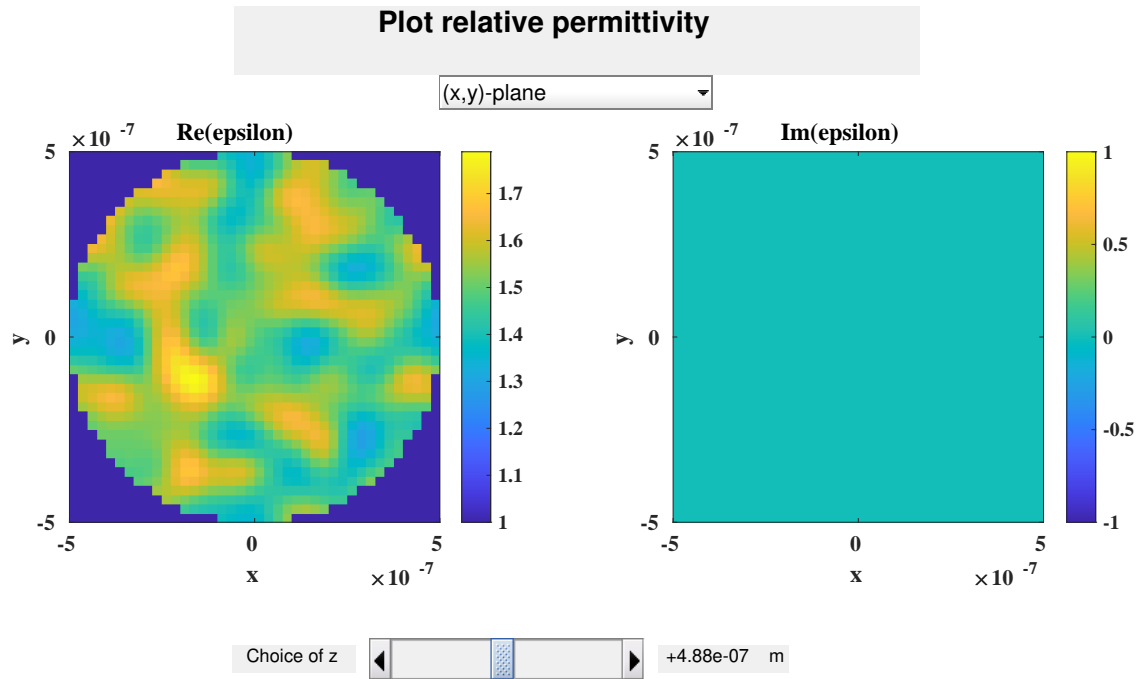


Figure 11.8 : Test2: relative permittivity. Real part (left) and imaginary part (right).

The following figures show the results obtained.

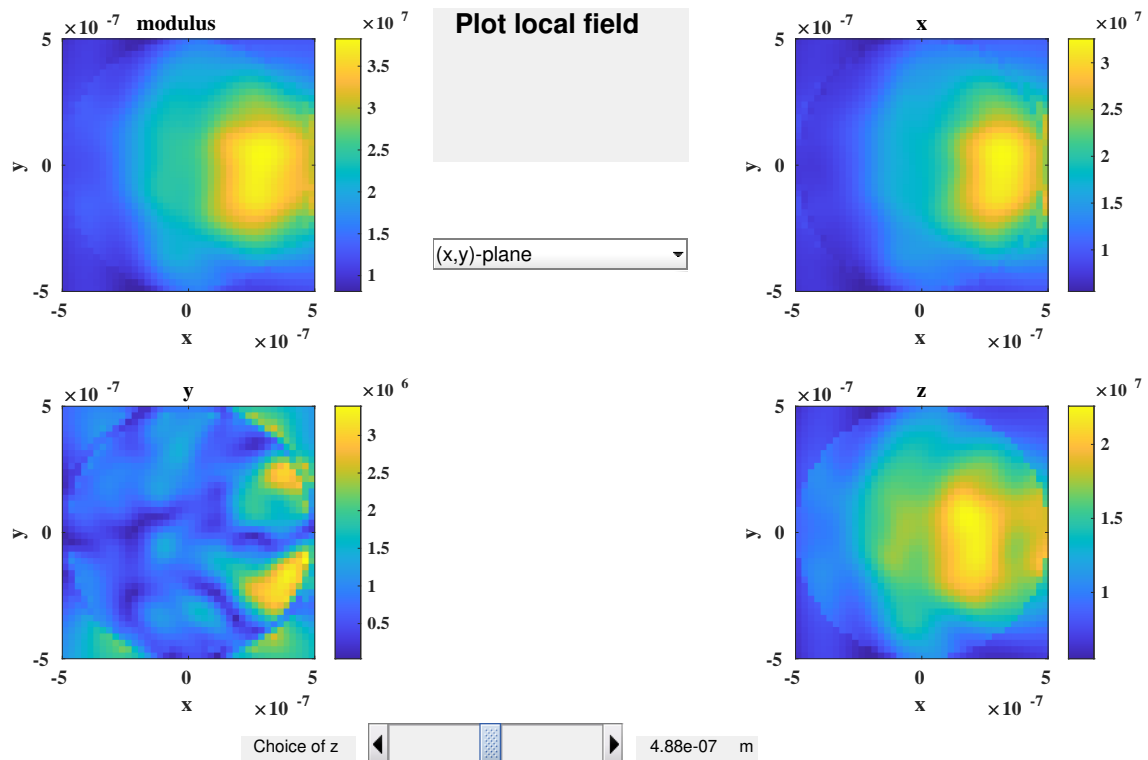


Figure 11.9 : Modulus of the local field in the (x,y) plane.

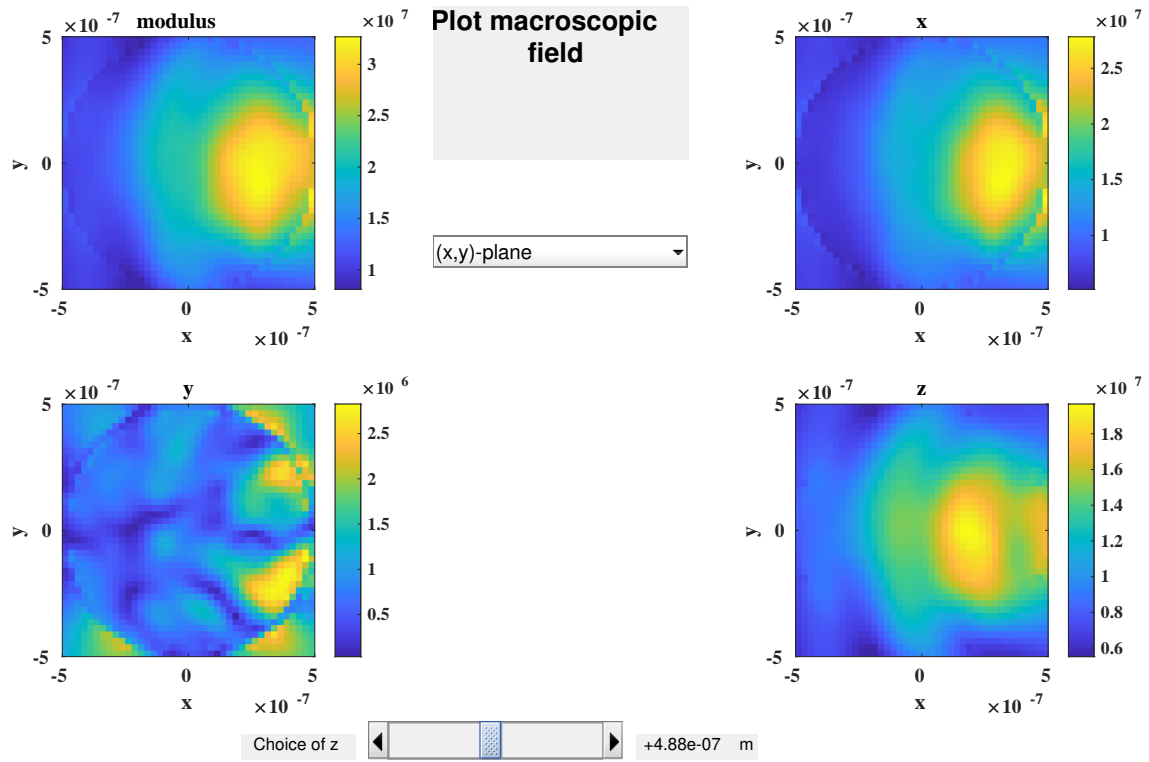


Figure 11.10 : Modulus of the macroscopic field in the (x, y) plane.

Poynting Modulus in k_x and k_y plane

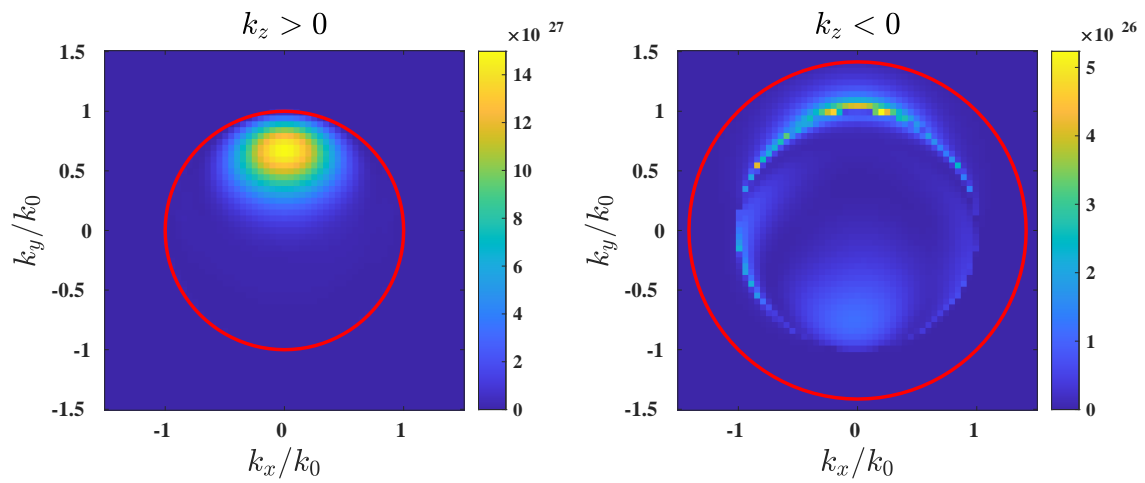


Figure 11.11 : Modulus of the Poynting vector.

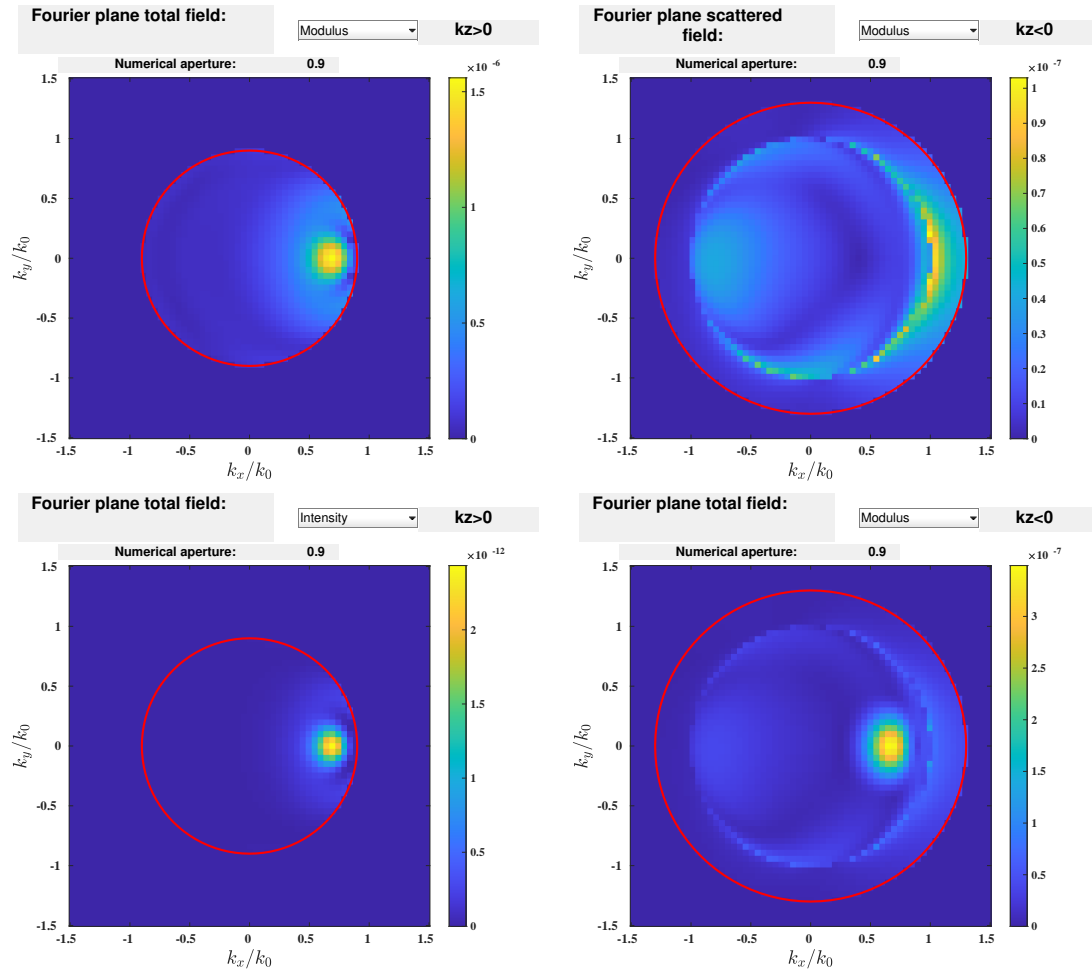


Figure 11.12 : Modulus of the field in the Fourier plane in transmission (left) and in reflection (right) for an optical diffraction tomography microscope. Diffracted field (above) and total field (below).

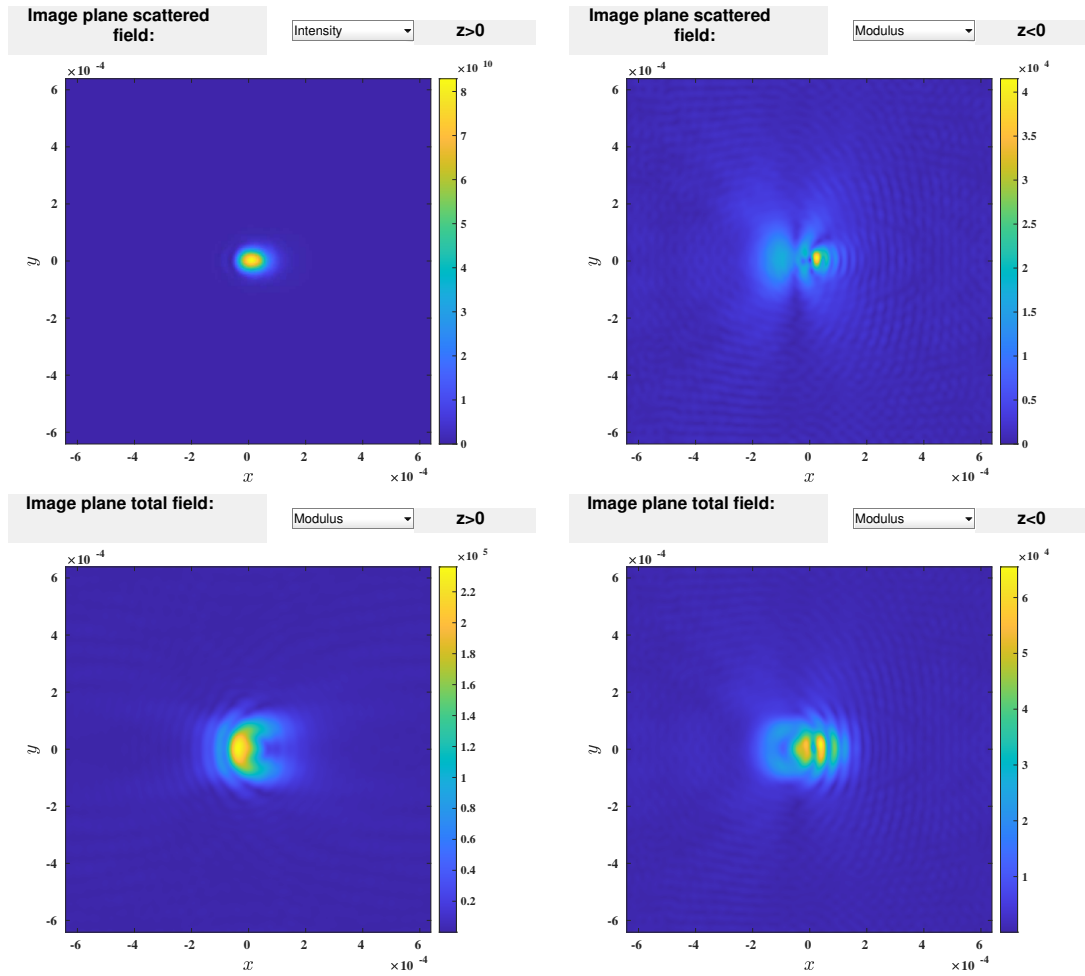


Figure 11.13 : Modulus of the field in the image plane in transmission (left) and in reflection (right) for an optical diffraction tomography microscope. Diffracted field (above) and total field (below).

11.4 Test3

The aim of the test3 is to test the brightfield microscope with a sphere of radius of 500 nm and a permittivity of 1.1 put upon a glass substrate ($\varepsilon = 2.25$).

Start calculation

Save configuration

Calculation options

Rigorous

Read local field from file

☐

Database file

Save in HDF5 file

Name h5 file

ifdda.h5

Advanced interface

☒

Illumination properties

Wavelength (nm)

632.8

P0 (W)

1

W0 (nm)

6328

Beam

Linear plane wave

Props

Number of plane waves

1

Multilayer properties

Number of interfaces

1

+

-

Props

Object properties

Object

sphere

Props

Number of objects

1

Anisotropy

iso

Epsilon

Discretization

30

Study

Only dipoles

☐

Far field

☐

Microscopy

☒

Type of Microscope:

Brightfield

Quick computation (FFT):

☒

Magnification factor:

100

Side Computation:

Both side

Numerical aperture: [0 n_l] (reflexion):

1.3

Position focal plane reflexion (nm):

300

Numerical aperture: [0 n₊] (transmission):

0.9

Position focal plane transmission (nm):

-100

Numerical aperture: [0 n_l] (condenser lens):

0.9

Near field

☐

Numerical parameters

Tolerance

0.0001

Methode

GPBICG1

Green functions

Level 2

Polarizability

RR

FFT

512

Figure 11.14 : Test3: configuration taken.

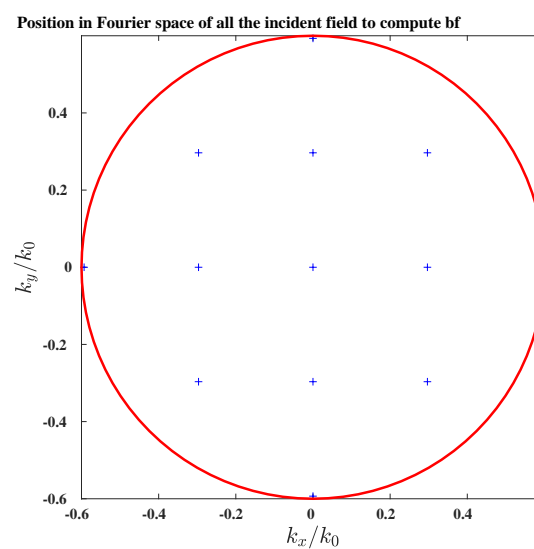


Figure 11.15 : Test3: Incident field used to simulate the microscope.

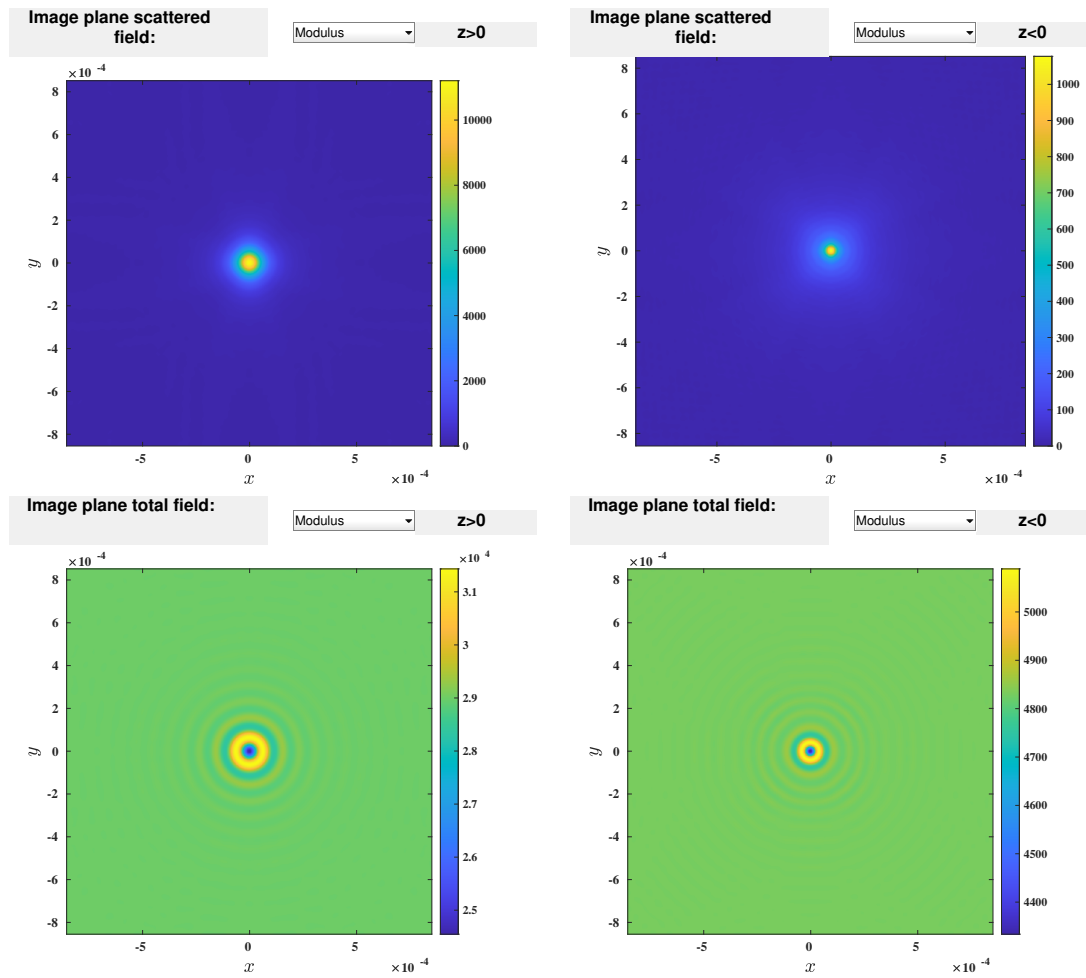


Figure 11.16 : *Modulus of the field in the image plane in case of transmission (left) and reflection (right) for a darkfield (above) and brightfield (below) microscope.*

11.5 Test4

The aim of test4 is to test the dark field and phase microscope with a sphere of radius of 500 nm and a permittivity of 1.1 put upon a glass substrate ($\varepsilon = 2.25$).

Start calculation

Save configuration

Calculation options

Rigorous

Read local field from file

☐

Database file

Save in HDF5 file

Name h5 file

ifdda.h5

Advanced interface

☒

Illumination properties

Wavelength (nm)

632.8

P0 (W)

1

W0 (nm)

6328

Beam

Linear plane wave

Props

Number of plane waves

1

Multilayer properties

Number of interfaces

1

+

-

Props

Object properties

Object

sphere

Props

Number of objects

1

Anisotropy

iso

Epsilon

Discretization

30

Study

Only dipoles

☐

Far field

☐

Microscopy

☒

Type of Microscope:

Darkfield & pha

Quick computation (FFT):

☒

Magnification factor:

100

Side Computation:

Both side

Numerical aperture: [0 n₊] (reflexion):

1.3

Position focal plane reflexion (nm):

300

Numerical aperture: [0 n₊] (transmission):

0.9

Position focal plane transmission (nm):

-100

Numerical aperture: [0 n₊] (condenser lens):

0.9

Near field

☐

Numerical parameters

Tolerance

0.0001

Methode

GPBICG1

Green functions

Level 2

Polarizability

RR

FFT

512

Figure 11.17 : Test3: configuration taken.

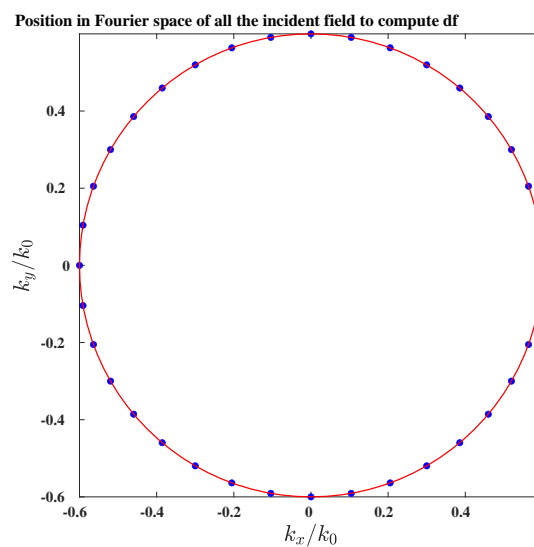


Figure 11.18 : Test4: Incident field used to simulate the microscope.

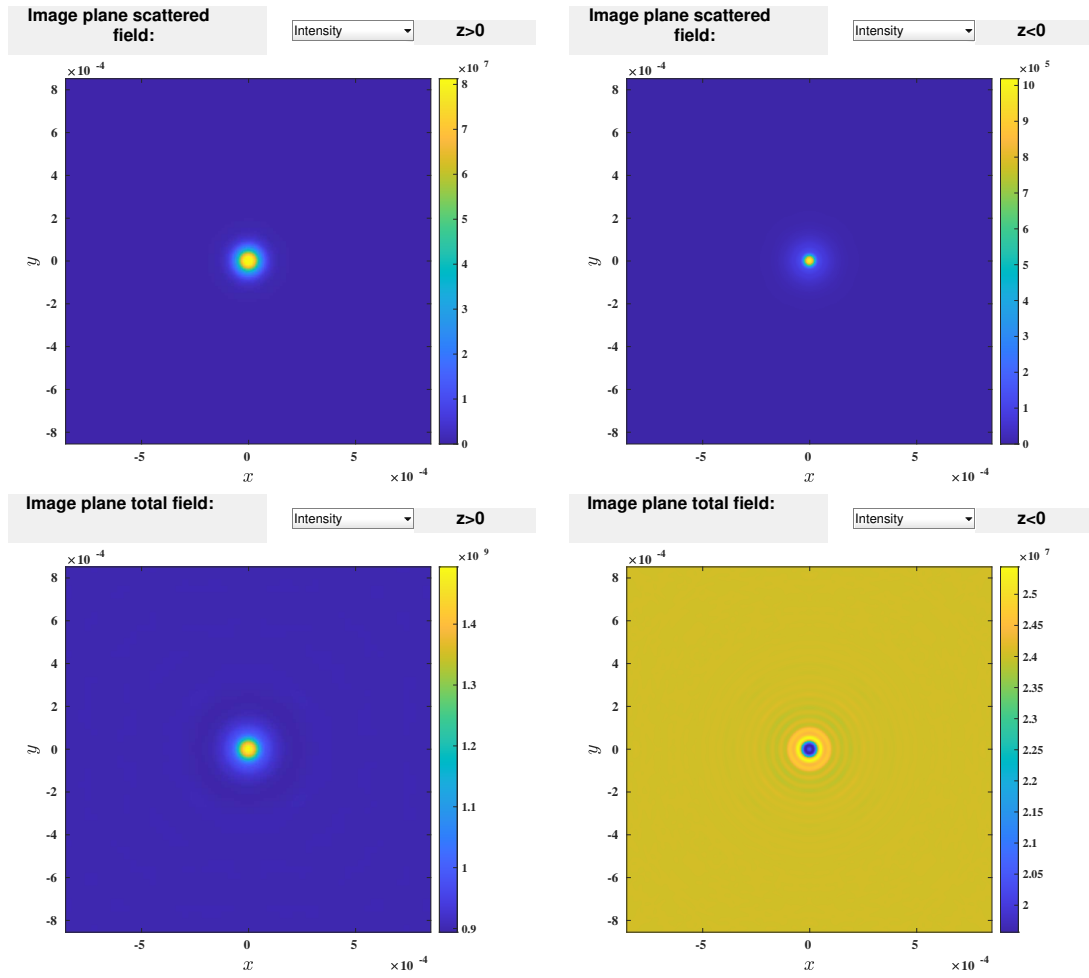


Figure 11.19 : Modulus of the field in the image plane in case of transmission (left) and reflection (right) for a darkfield (above) and phase (below) microscope.

Bibliography

- [1] F. M. Kahnert, J. Quant. Spect. Rad. Transf. **79-80**, 775 (2003).
- [2] E. M. Purcell and C. R. Pennypacker, Astrophys. J. **186**, 705 (1973).
- [3] B. T. Draine, Astrophys. J. **333**, 848 (1988).
- [4] P. C. Chaumet, A. Sentenac, and A. Rahmani, Phys. Rev. E **70**, 036606 (2004).
- [5] A. D. Yaghjian, Proceedings of the IEEE **68**, 248 (1980), ISSN 0018-9219.
- [6] M. Paulus, P. Gay-Balmaz, and O. J. F. Martin, Phys. Rev. E **62**, 5797 (2000).
- [7] G. H. Goedecke and S. G. O'Brien, Appl. Opt. **27**, 2431 (1988).
- [8] A. Lakhtakia, Int. J. Mod. Phys. C **3**, 583 (1992).
- [9] B. T. Draine and J. Goodman, Astrophys. J. **405**, 685 (1993).
- [10] A. Rahmani, P. C. Chaumet, and G. W. Bryant, Astrophys. J. **607**, 873 (2004).
- [11] P. C. Chaumet and A. Rahmani, Opt. Lett. **34**, 917 (2009).
- [12] M. Thuthu, S. Fujino, and Y. Onoue, IMECS **1** (2009).
- [13] S. Fujino and T. Sekimoto, IMECS **2** (2012).
- [14] R. D. Da Cunha and T. Hopkins, Appl. Numer. Math. **19**, 33 (1995).
- [15] T. F. Chan, E. Gallopoulos, V. Simoncini, T. Szeto, and C. H. Tong, SIAM J. Sci. Comput. **15**, 338 (1994).
- [16] L. Zhao, T.-Z. Huang, Y.-F. Jing, and L.-J. Deng, Computers & Mathematics with Applications **66**, 1372 (2013), ISSN 0898-1221.
- [17] B. Carpentieri, Y.-F. Jing, T.-Z. Huang, W.-C. Pi, and X.-Q. Sheng, Computational Electromagnetics International Workshop pp. 85–90 (2011).
- [18] S. Fujino and K. Iwasato, Proc. of the World Congress on Engineering **1** (2015).
- [19] T. F. Chan, SIAM Journal on Scientific and Statistical Computing **9**, 766 (1988).
- [20] S. P. Groth, A. G. Polimeridis, and J. K. White, Journal of Quantitative Spectroscopy and Radiative Transfer **240**, 106689 (2020), ISSN 0022-4073, URL <https://www.sciencedirect.com/science/article/pii/S0022407319302080>.

- [21] G. P. Agrawal and D. N. Pattanayak, J. Opt. Soc. Am. A **69**, 575 (1979).
- [22] A. Rahmani, P. C. Chaumet, F. de Fornel, and C. Girard, Phys. Rev. A **56**, 3245 (1997).
- [23] A. Rahmani, P. C. Chaumet, and F. de Fornel, Phys. Rev. A **63**, 023819 (2001).
- [24] E. Abbe, Journal of the Royal Microscopical Society **1**, 388 (1981).
- [25] S. Khadir, P. C. Chaumet, G. Baffou, and A. Sentenac, J. Opt. Soc. Am. A **36**, 478 (2019).